


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030215\
 Data File : BF077520.D
 Acq On : 2 Mar 2015 11:24
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 02 17:05:52 2015

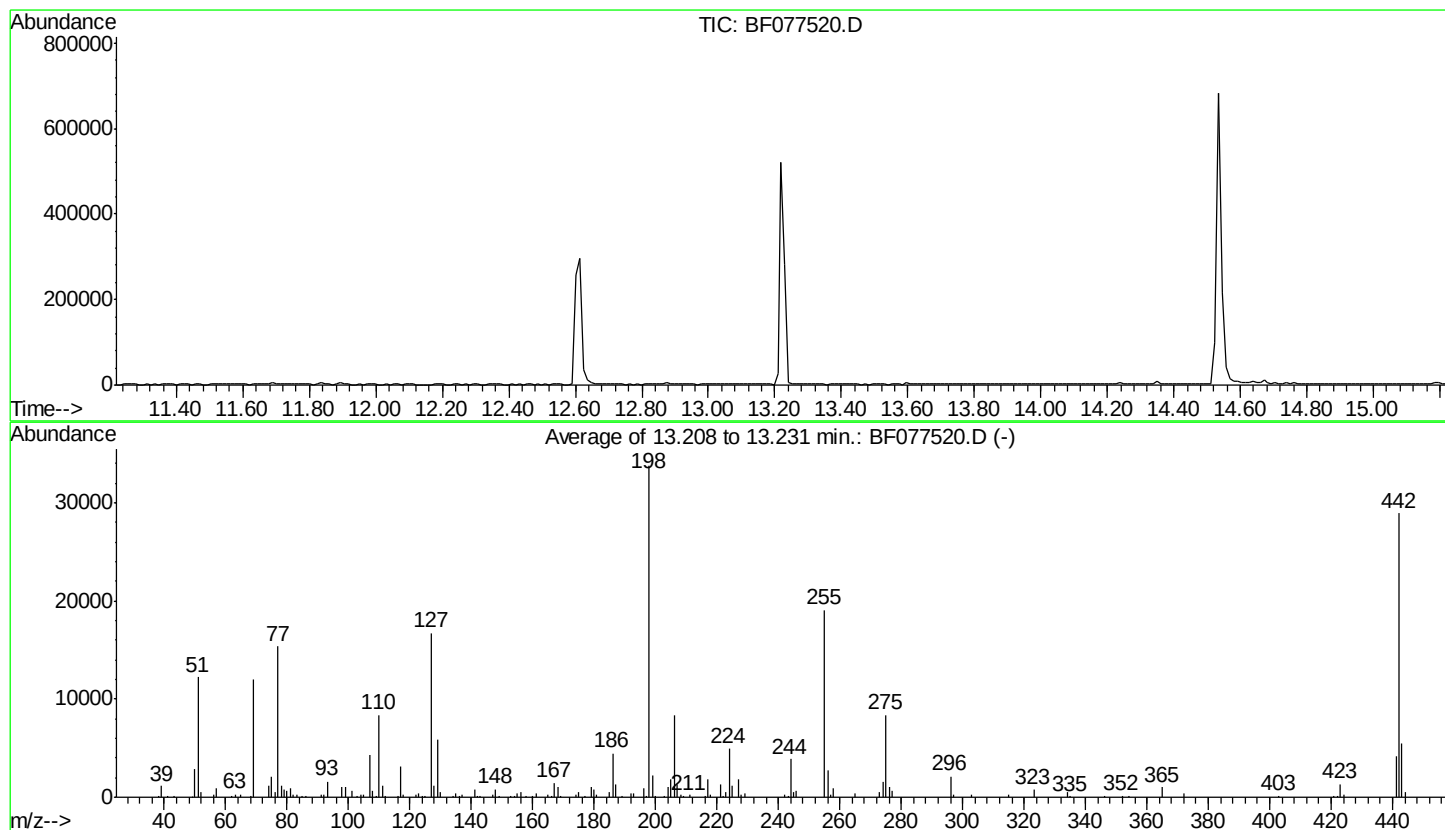

AutoFind: Scans 1078, 1079, 1080; Background Corrected with Scan 1075

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	12197	PASS
68	69	0.00	2	1.5	180	PASS
69	198	0.00	100	35.5	11987	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.5	16734	PASS
197	198	0.00	2	0.4	149	PASS
198	198	100	100	100.0	33777	PASS
199	198	5	9	6.4	2167	PASS
275	198	10	60	24.9	8408	PASS
365	198	1	100	2.9	994	PASS
441	442	0.01	24	14.7	4236	PASS
442	198	50	100	85.5	28896	PASS
443	442	15	24	19.1	5510	PASS