
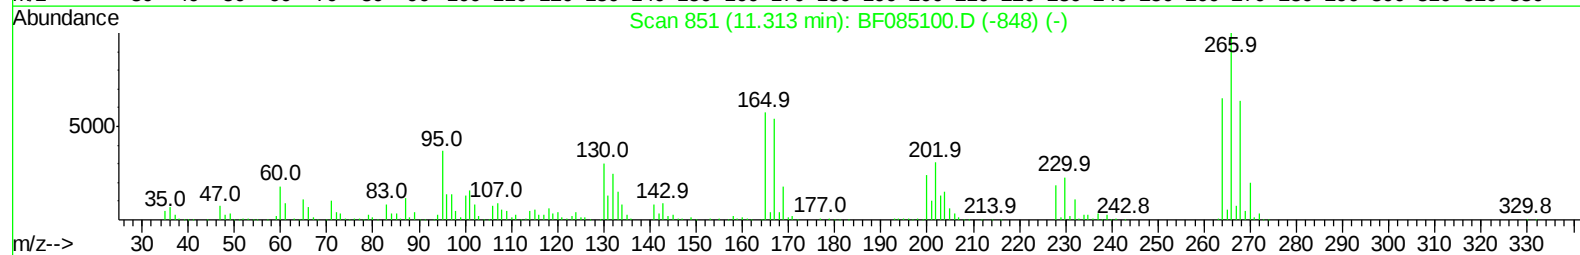
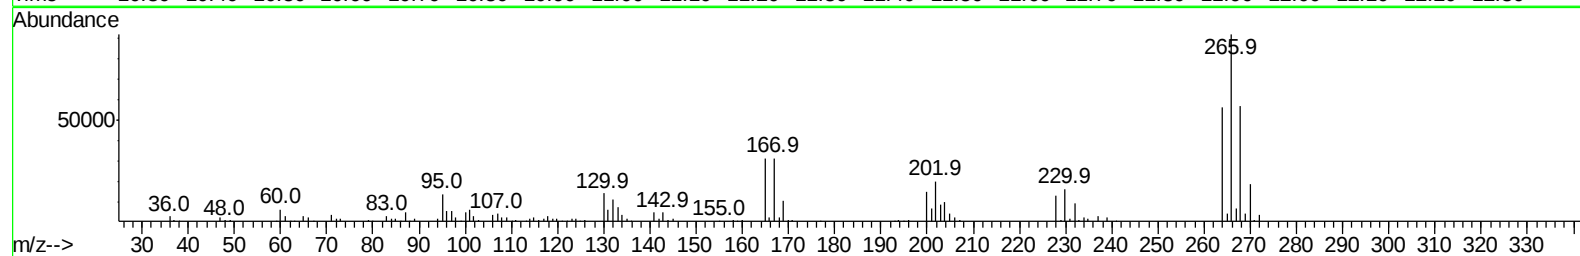


Data Path : Z:\HPCHEM1\BNA F\Data\BF030216\
Data File : BF085105.D
Acq On : 2 Mar 2016 8:33
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 06:54:36 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 02 13:25:39 2016
Response via : Initial Calibration

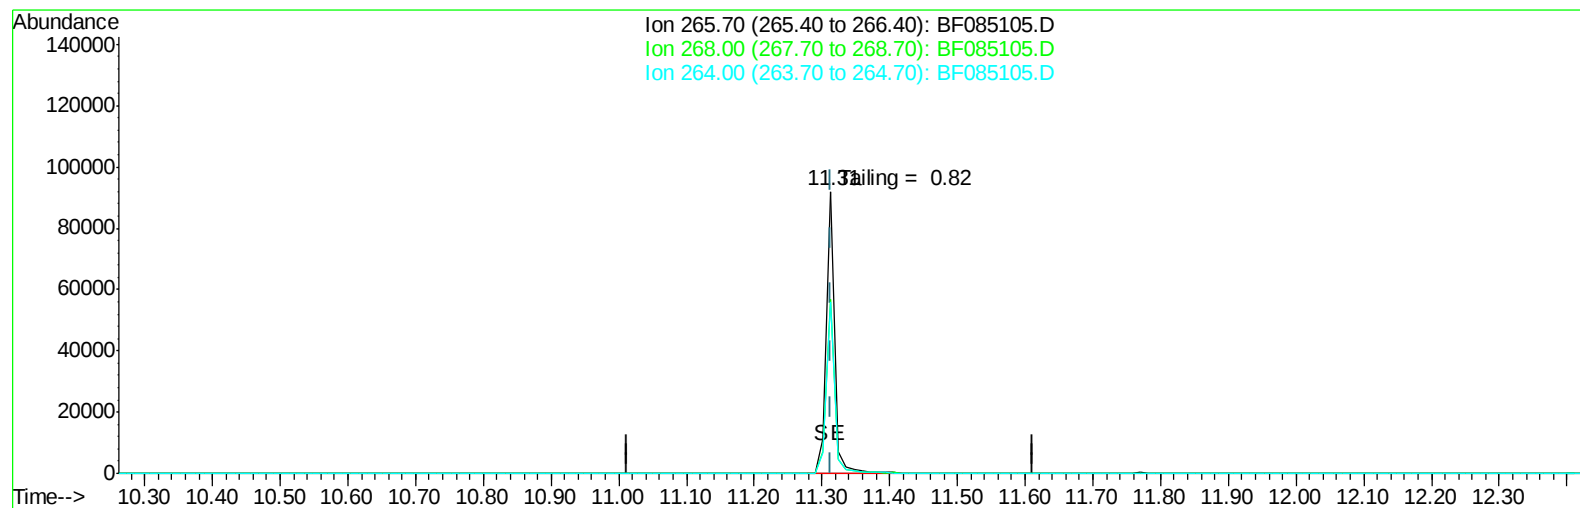

TIC: BF085105.D

(69) Pentachlorophenol (C)




11.313min (+0.000) 0.00ng

response 79705

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	61.99
264.00	65.40	61.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF030216\
Data File : BF085105.D
Acq On : 2 Mar 2016 8:33
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 06:54:36 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF030116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 02 13:25:39 2016
Response via : Initial Calibration

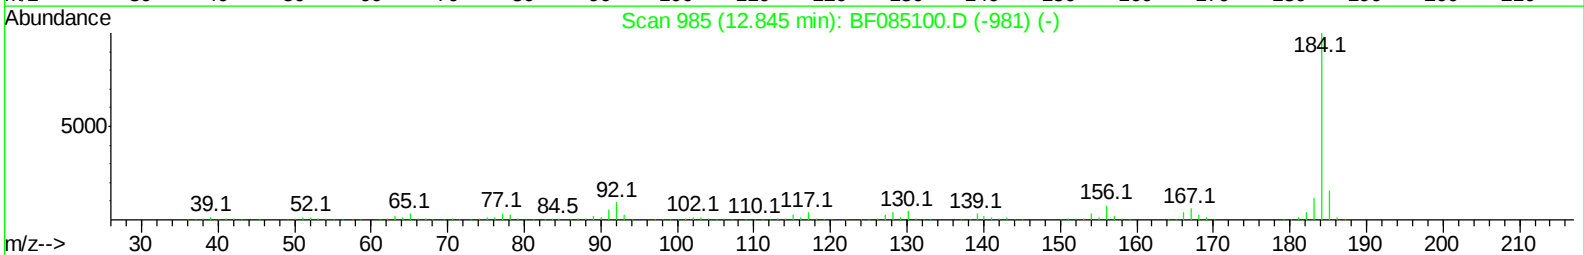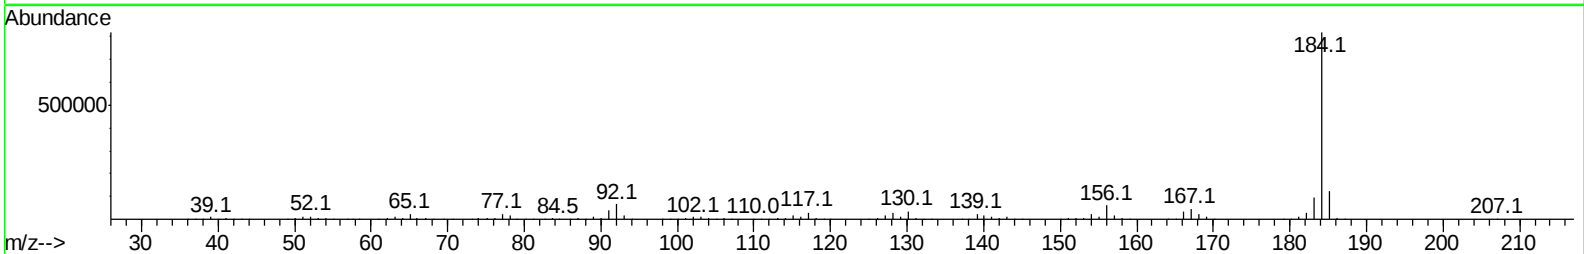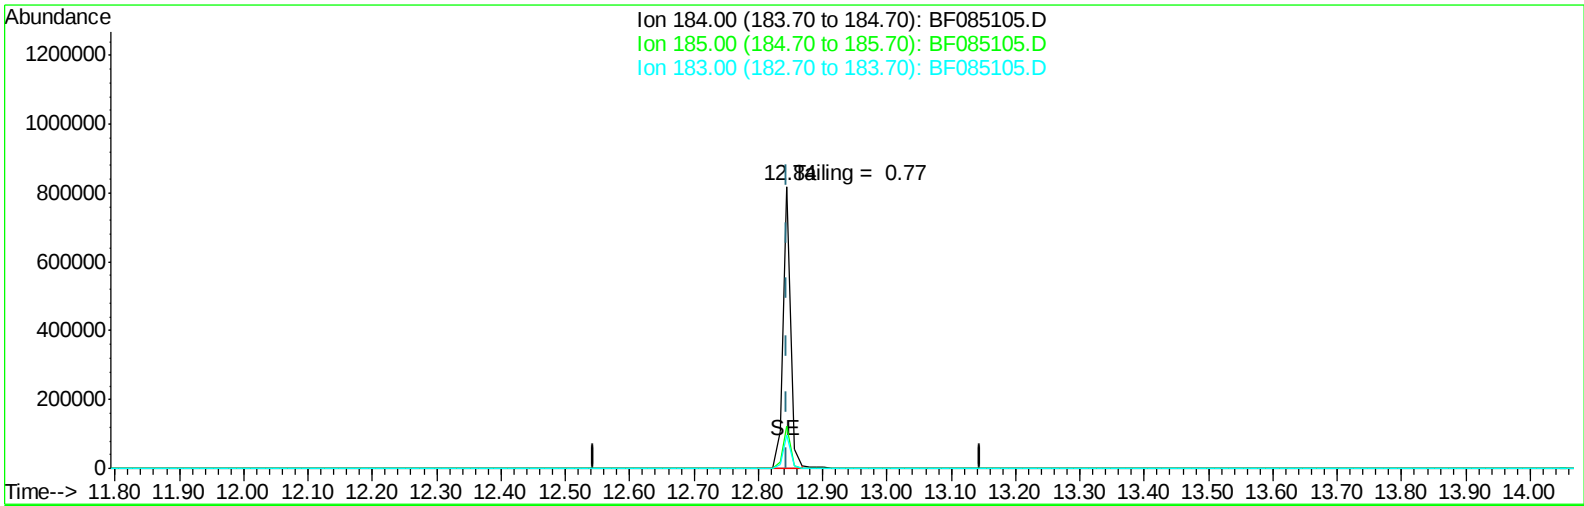

TIC: BF085105.D

(76) Benzidine

12.845min (-0.000) 93875.56ng

response 695353

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.95
183.00	11.90	11.69
0.00	0.00	0.00