


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030216\
 Data File : BF085105.D
 Acq On : 2 Mar 2016 8:33
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 02 13:25:39 2016

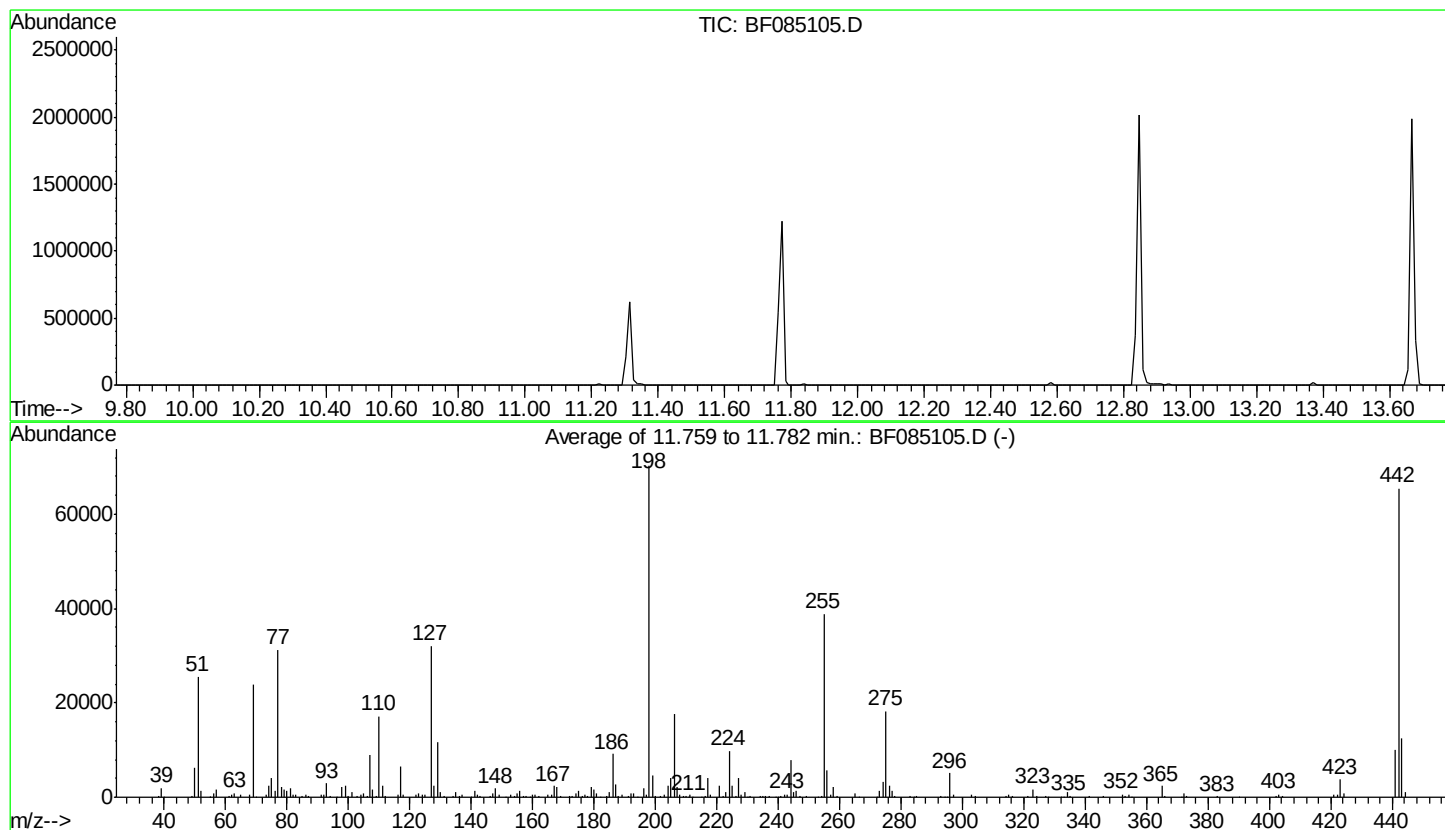

AutoFind: Scans 890, 891, 892; Background Corrected with Scan 886

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	25554	PASS
68	69	0.00	2	1.8	437	PASS
69	198	0.00	100	34.0	23912	PASS
70	69	0.00	2	0.4	103	PASS
127	198	10	80	45.7	32106	PASS
197	198	0.00	2	0.6	440	PASS
198	198	100	100	100.0	70310	PASS
199	198	5	9	6.8	4749	PASS
275	198	10	60	26.0	18251	PASS
365	198	1	100	3.4	2405	PASS
441	442	0.01	24	15.3	9997	PASS
442	198	50	100	93.1	65466	PASS
443	442	15	24	19.2	12553	PASS