


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030216\
 Data File : BF085129.D
 Acq On : 2 Mar 2016 19:51
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 02 13:25:39 2016

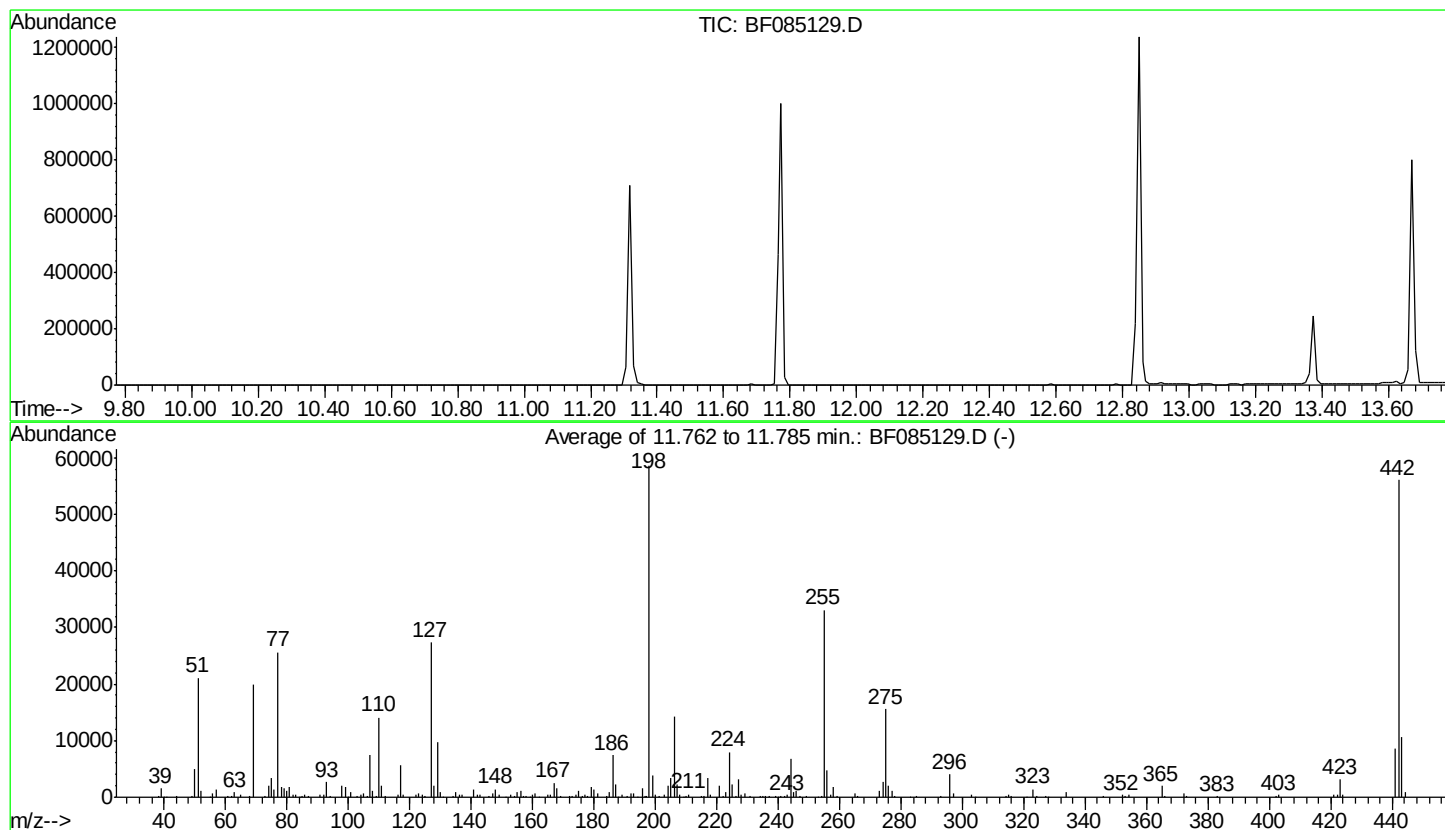

AutoFind: Scans 829, 830, 831; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	21114	PASS
68	69	0.00	2	1.5	307	PASS
69	198	0.00	100	33.9	19853	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.7	27333	PASS
197	198	0.00	2	0.6	327	PASS
198	198	100	100	100.0	58572	PASS
199	198	5	9	6.6	3853	PASS
275	198	10	60	26.6	15571	PASS
365	198	1	100	3.4	1968	PASS
441	442	0.01	24	15.5	8672	PASS
442	198	50	100	95.7	56073	PASS
443	442	15	24	19.2	10741	PASS