
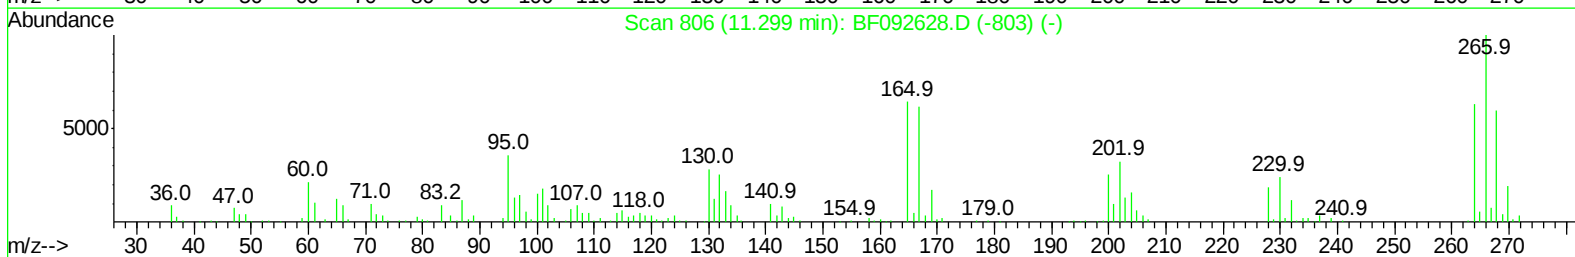
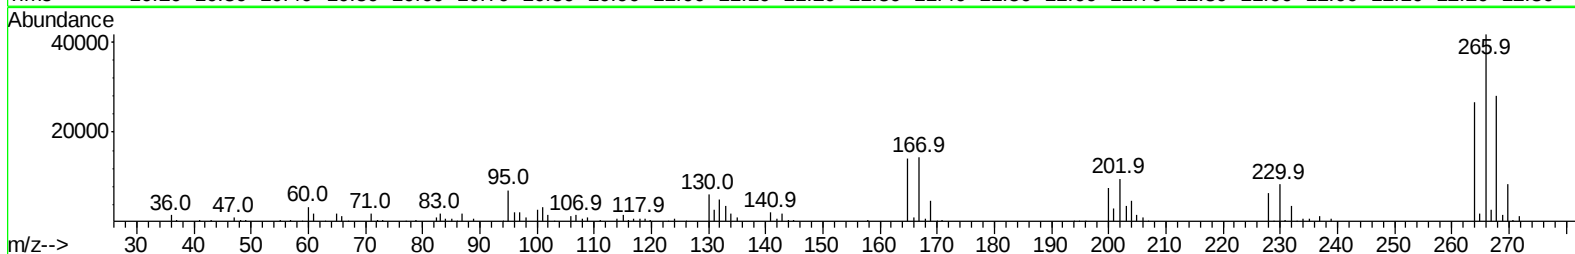


Data Path : Z:\HPCHEM1\BNA F\DATA\BF030217\
Data File : BF093348.D
Acq On : 3 Mar 2017 8:22
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 09:45:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

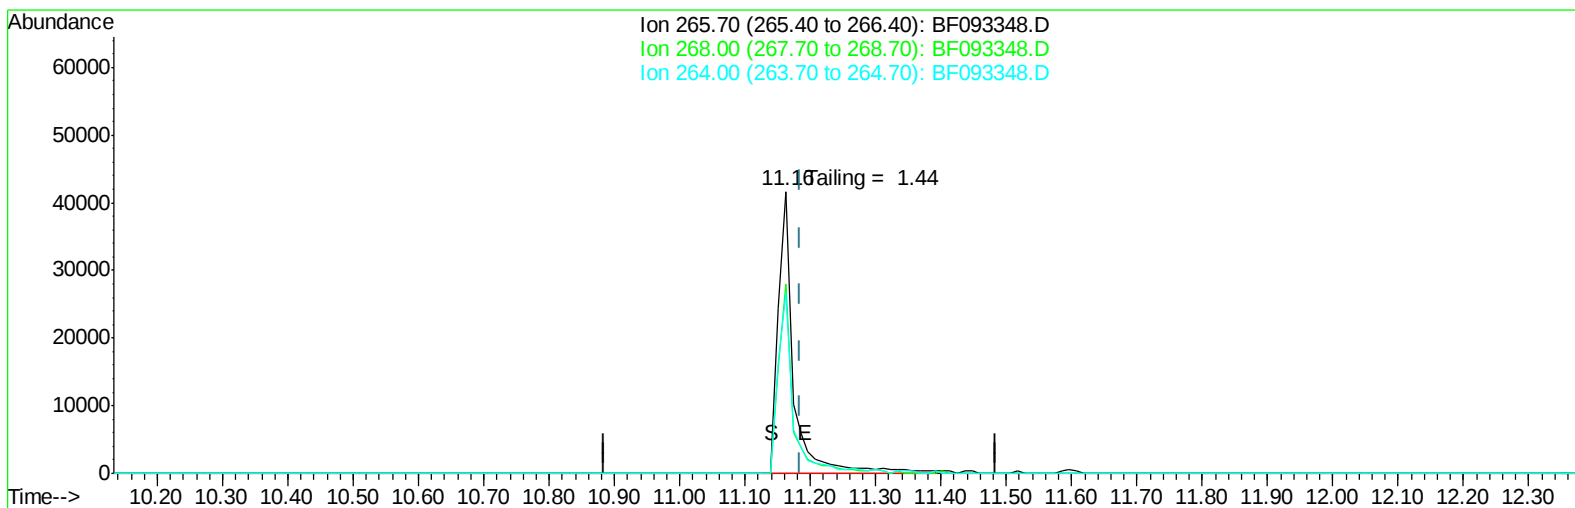

TIC: BF093348.D

(69) Pentachlorophenol (C)




11.162min (-0.023) 19003.71ng

response 67981

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	67.22
264.00	62.90	63.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030217\
Data File : BF093348.D
Acq On : 3 Mar 2017 8:22
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 09:45:36 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

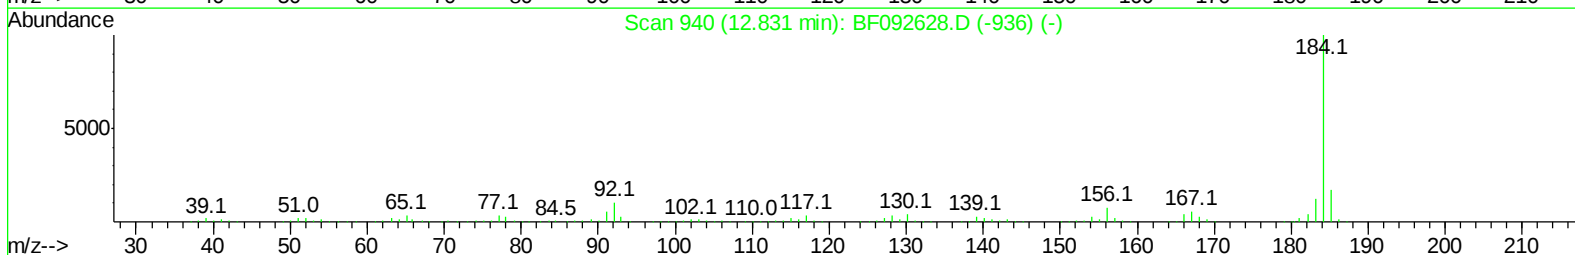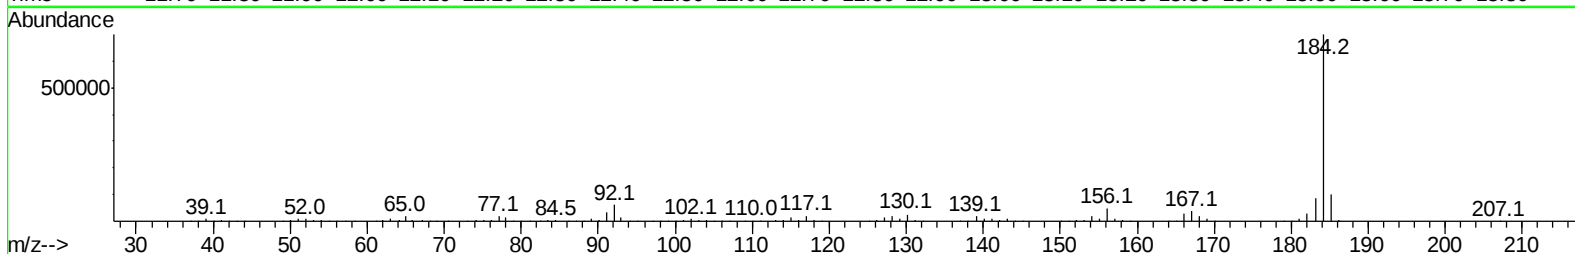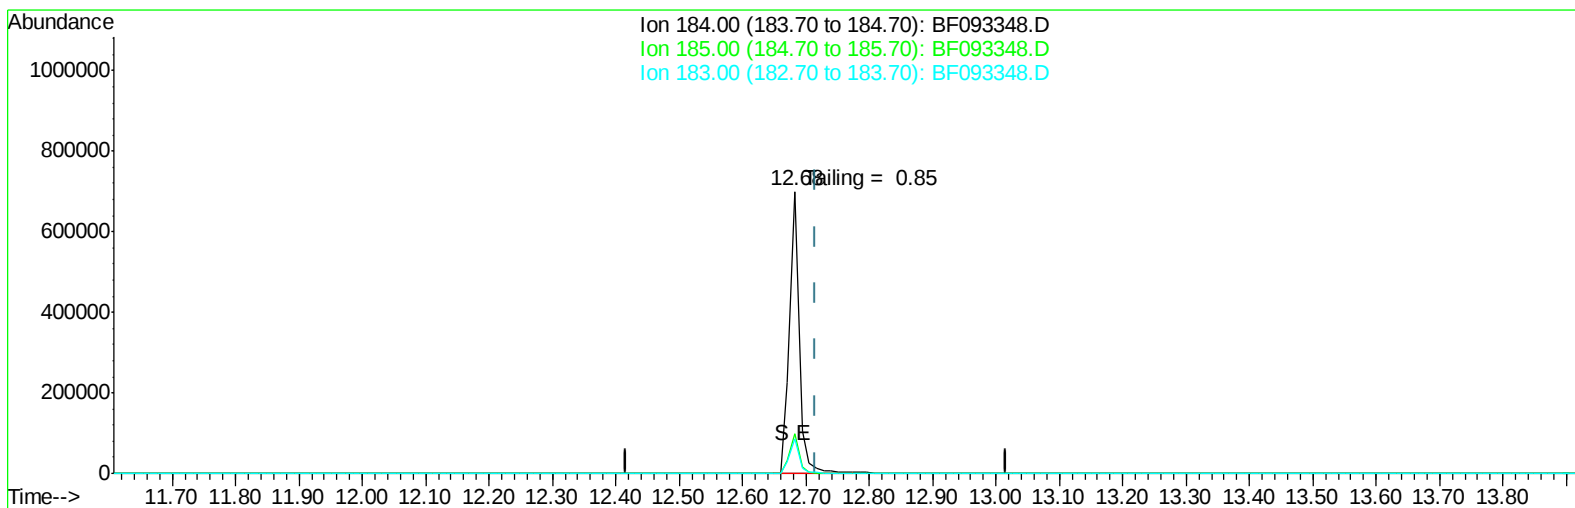

TIC: BF093348.D

(76) Benzidine

12.682min (-0.034) 5690.67ng

response 760221

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.22
183.00	11.50	12.27
0.00	0.00	0.00