


Data Path : Z:\HPCHEM1\BNA F\Data\BF030217\
 Data File : BF093322.D
 Acq On : 2 Mar 2017 15:40
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 17:31:55 2017

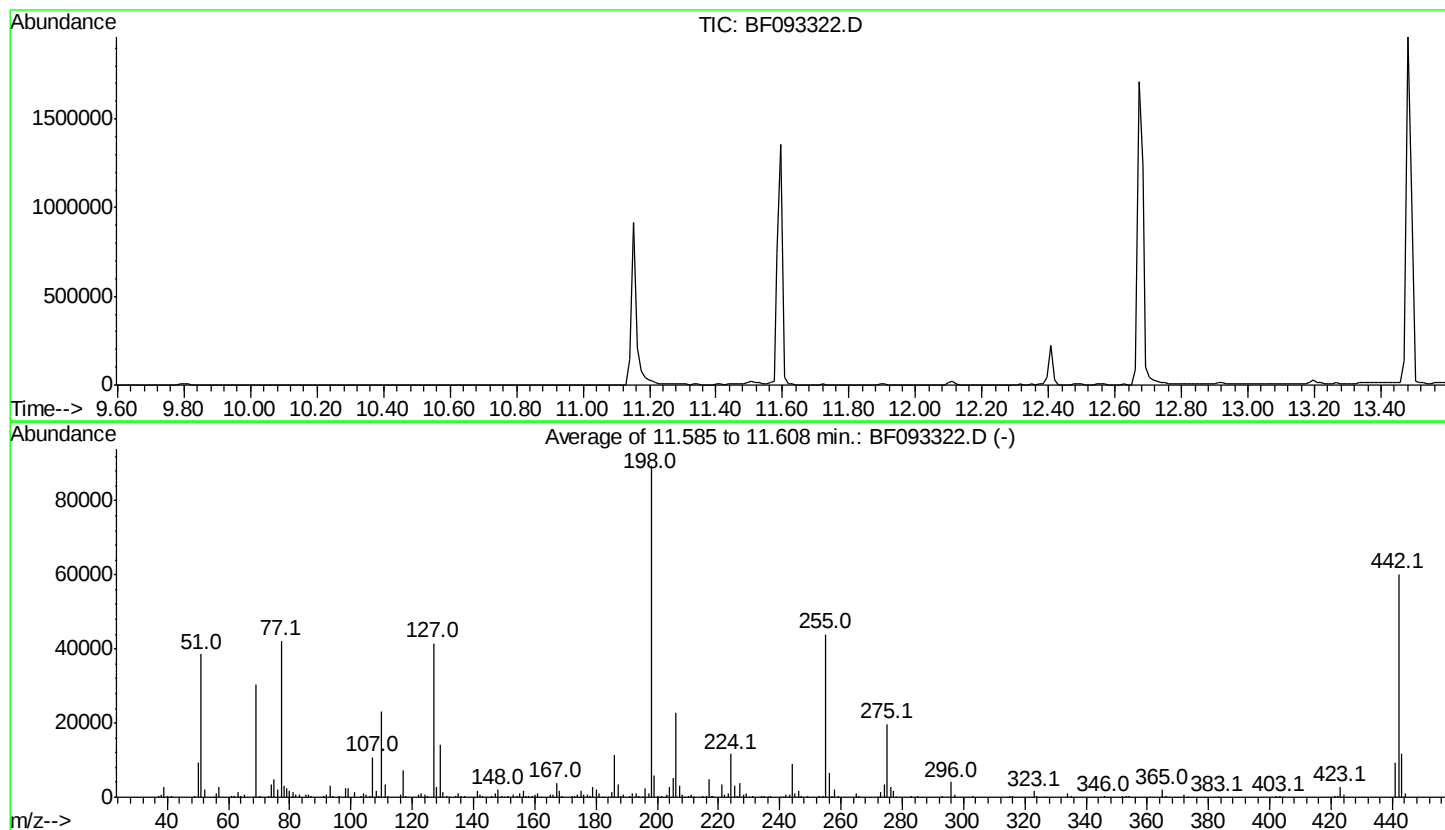

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	38664	PASS
68	69	0.00	2	0.5	141	PASS
69	198	0.00	100	33.9	30332	PASS
70	69	0.00	2	0.8	249	PASS
127	198	10	80	46.5	41603	PASS
197	198	0.00	2	1.2	1058	PASS
198	198	100	100	100.0	89477	PASS
199	198	5	9	6.8	6042	PASS
275	198	10	60	22.2	19866	PASS
365	198	1	100	2.2	1950	PASS
441	442	0.01	24	15.6	9427	PASS
442	198	50	100	67.3	60247	PASS
443	442	15	24	19.3	11598	PASS