


Data Path : Z:\HPCHEM1\BNA F\DATA\BF030217\
 Data File : BF093348.D
 Acq On : 3 Mar 2017 8:22
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 17:31:55 2017

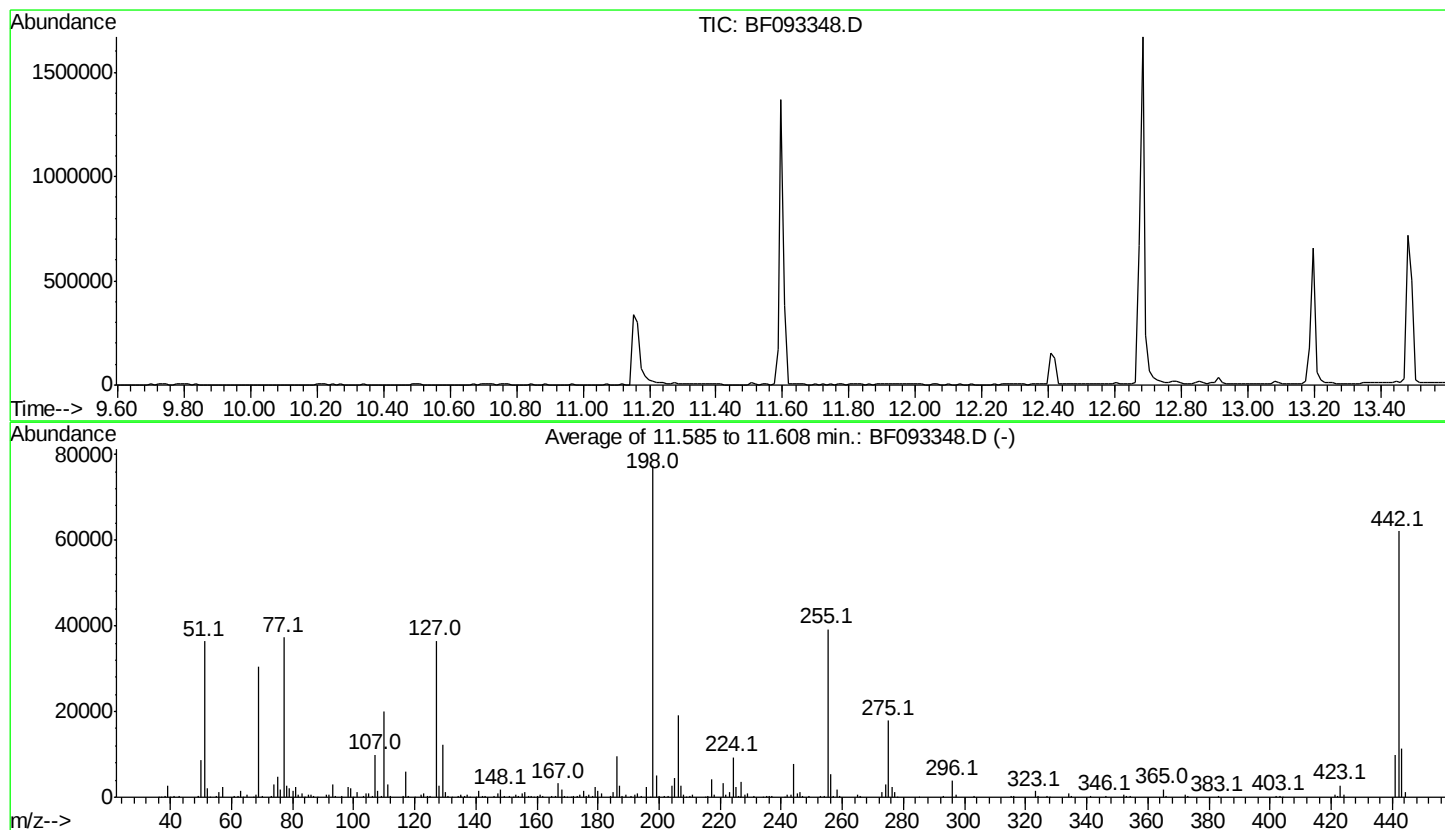

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	36387	PASS
68	69	0.00	2	2.0	598	PASS
69	198	0.00	100	39.3	30412	PASS
70	69	0.00	2	0.5	165	PASS
127	198	10	80	47.1	36482	PASS
197	198	0.00	2	0.2	145	PASS
198	198	100	100	100.0	77384	PASS
199	198	5	9	6.6	5111	PASS
275	198	10	60	23.1	17849	PASS
365	198	1	100	2.3	1801	PASS
441	442	0.01	24	16.1	9960	PASS
442	198	50	100	80.1	62023	PASS
443	442	15	24	18.2	11262	PASS