
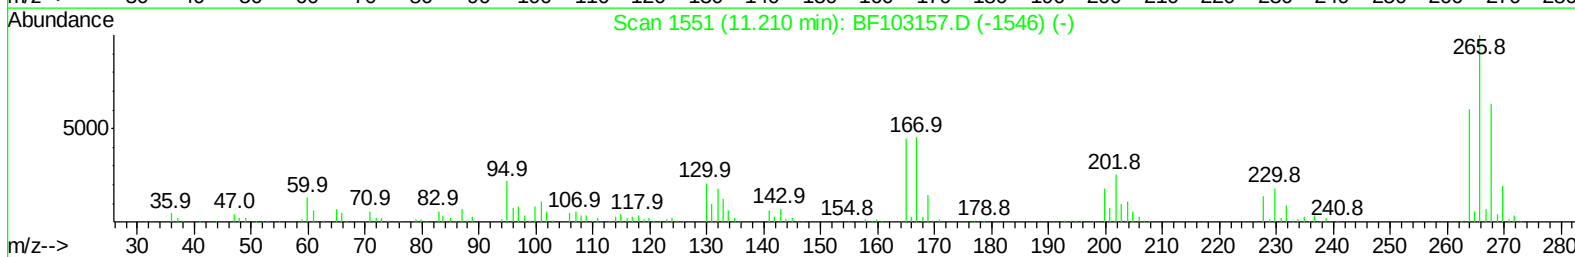
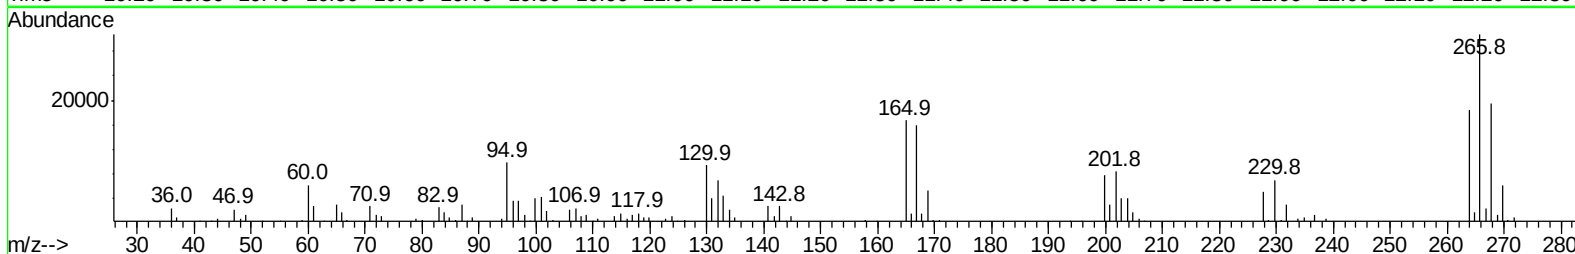


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030218\
Data File : BF103354.D
Acq On : 2 Mar 2018 9:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 01:09:28 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 02 13:28:09 2018
Response via : Initial Calibration

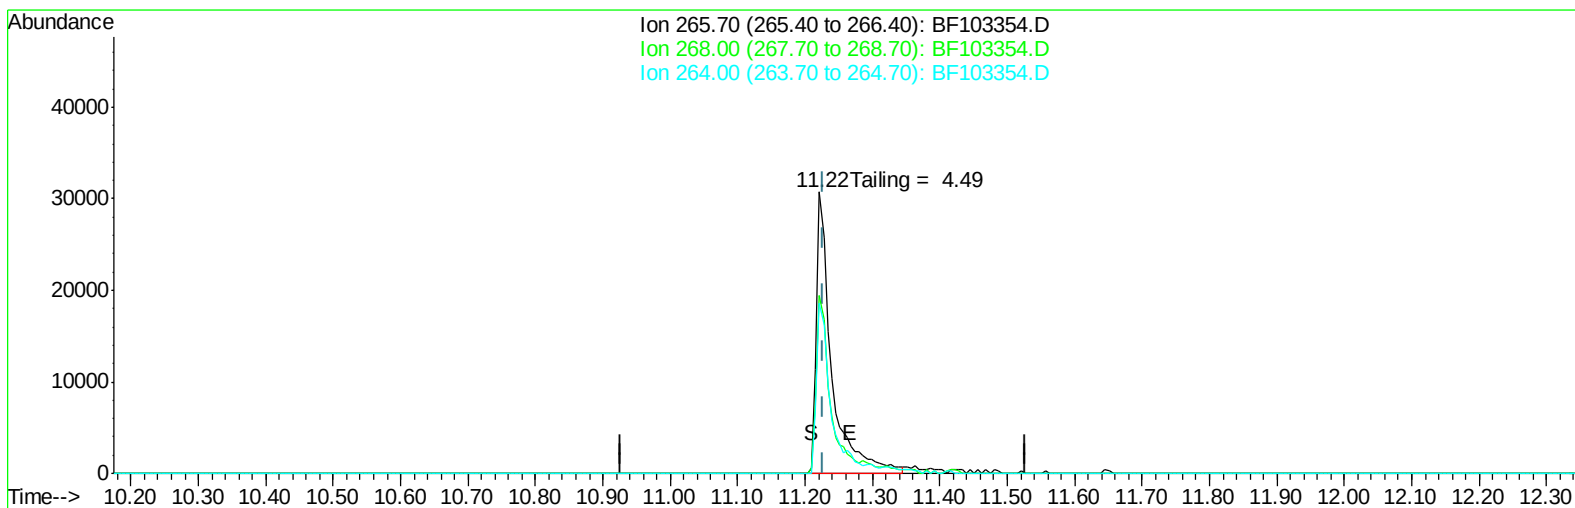

TIC: BF103354.D

(69) Pentachlorophenol (C)




11.222min (-0.006) 50119.36ng

response 47402

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.28
264.00	61.90	60.29
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030218\
 Data File : BF103354.D
 Acq On : 2 Mar 2018 9:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 01:09:28 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 02 13:28:09 2018
 Response via : Initial Calibration

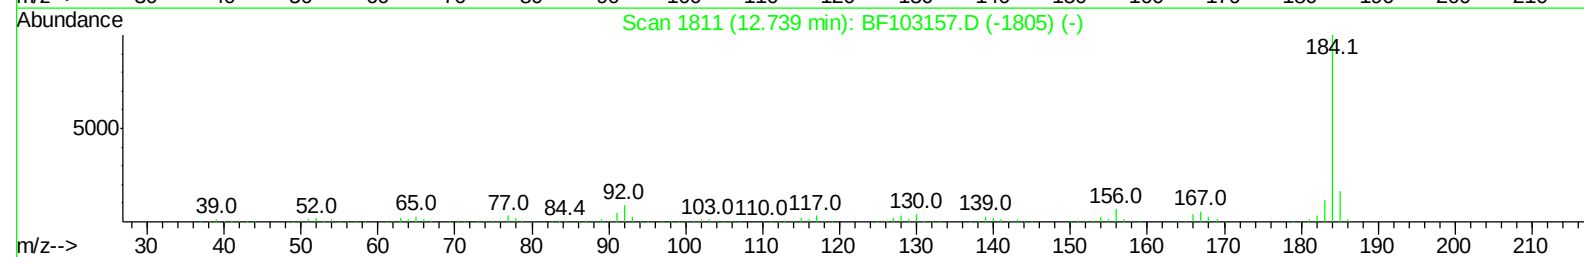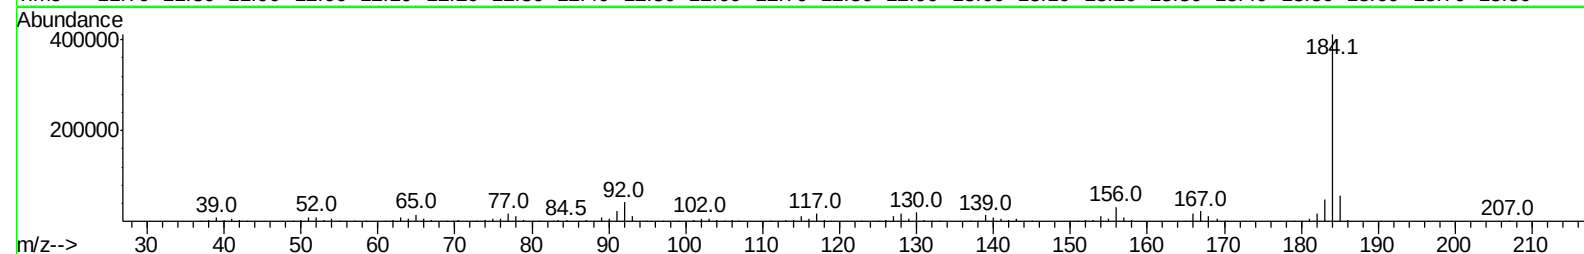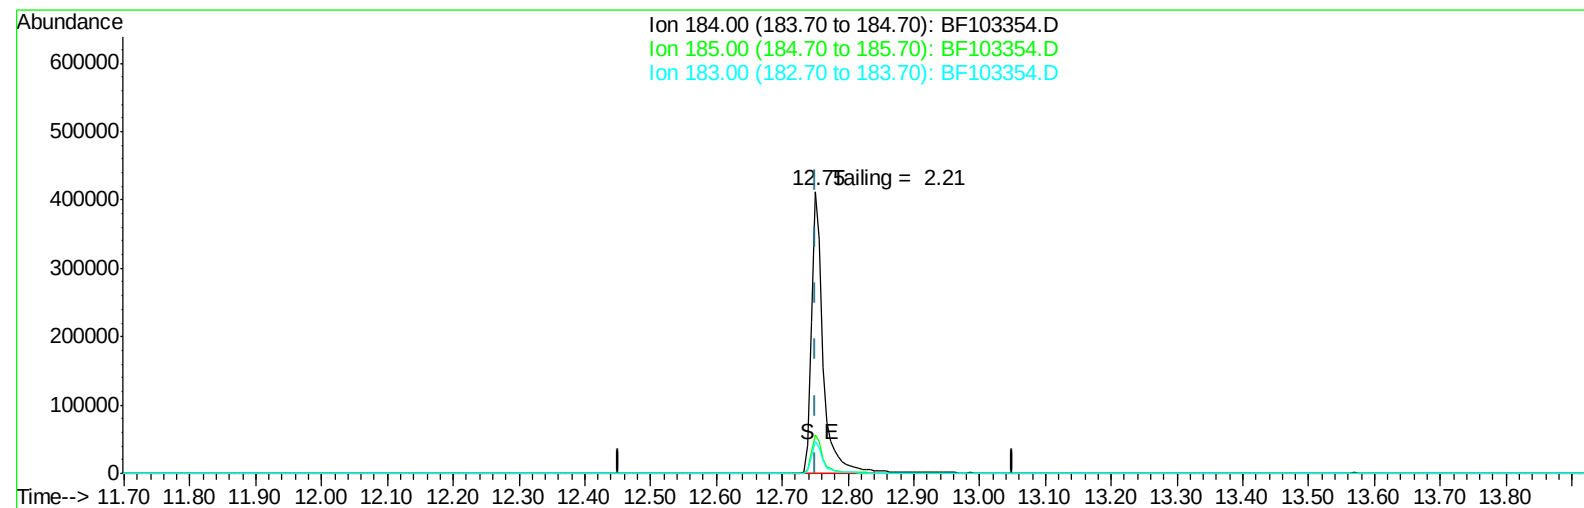

TIC: BF103354.D

(76) Benzidine

12.751min (+0.000) 0.00ng

response 518567

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.76
183.00	11.60	11.57
0.00	0.00	0.00