

Data Path : Z:\HPCHEM1\BNA_F\Data\BF030218\
 Data File : BF103359.D
 Acq On : 2 Mar 2018 11:58
 Operator : SJ/JU
 Sample : PB106993BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB106993BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.128	4	7	18	rVB2	27630	55902	4.66%	0.578%
2	5.498	577	580	598	rBV	330818	478017	39.88%	4.939%
3	6.510	749	752	766	rBV	273503	444532	37.08%	4.593%
4	6.645	772	775	788	rVB	524621	505066	42.13%	5.218%
5	6.875	810	814	825	rBV	880065	802062	66.91%	8.287%
6	7.028	836	840	854	rVB	422957	402416	33.57%	4.158%
7	7.439	907	910	924	rBV	201713	291282	24.30%	3.009%
8	8.157	1028	1032	1048	rBV	1007408	1107463	92.39%	11.442%
9	9.233	1211	1215	1226	rBV	446925	538335	44.91%	5.562%
10	9.916	1327	1331	1349	rBV	1057730	1198726	100.00%	12.385%
11	10.716	1464	1467	1476	rBV	110197	138311	11.54%	1.429%
12	11.410	1581	1585	1604	rBV	1116855	1178350	98.30%	12.174%
13	12.992	1850	1854	1863	rBV	587212	556446	46.42%	5.749%
14	14.062	2032	2036	2048	rBV	920169	1029503	85.88%	10.637%
15	14.821	2161	2165	2168	rBV3	20454	29554	2.47%	0.305%
16	15.162	2220	2223	2226	rBV	25715	28699	2.39%	0.297%
17	15.574	2286	2293	2304	rBV	488153	854512	71.29%	8.829%
18	15.998	2361	2365	2371	rVB2	25761	39738	3.32%	0.411%


Sum of corrected areas: 9678914

Data Path : Z:\HPCHEM1\BNA_F\Data\BF030218\
Data File : BF103359.D
Acq On : 2 Mar 2018 11:58
Operator : SJ/JU
Sample : PB106993BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB106993BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

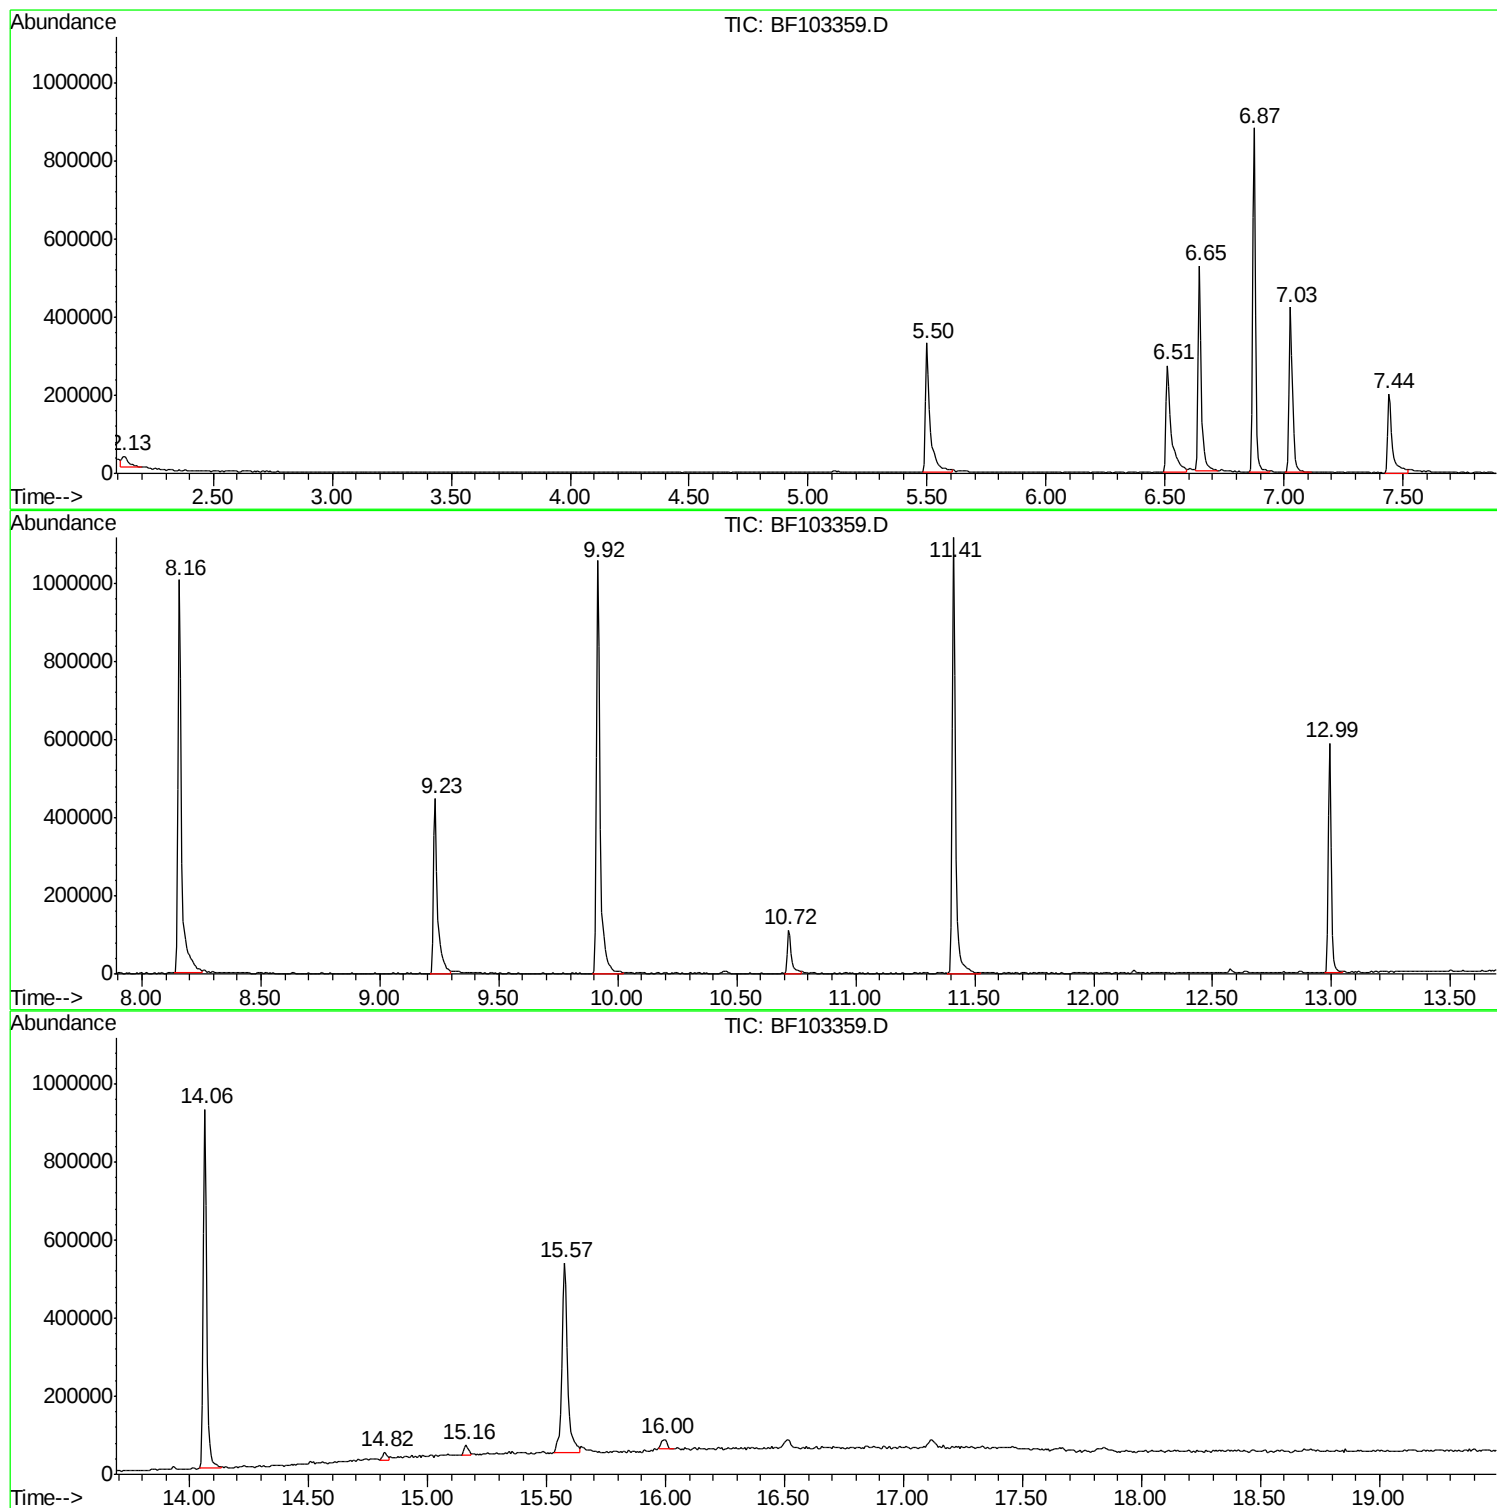

Data Path : Z:\HPCHEM1\BNA F\Data\BF030218\
Data File : BF103359.D
Acq On : 2 Mar 2018 11:58
Operator : SJ/JU
Sample : PB106993BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB106993BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.65	12.59 ng	505066	1,4-Dichlorobenzene-d4	6.87

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

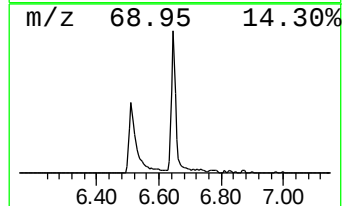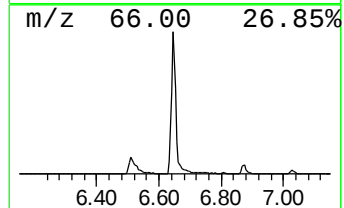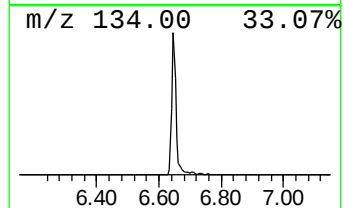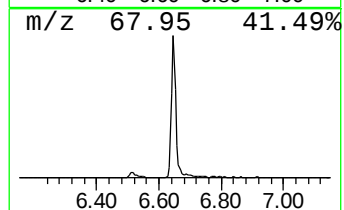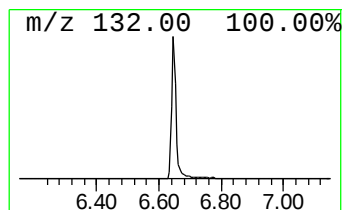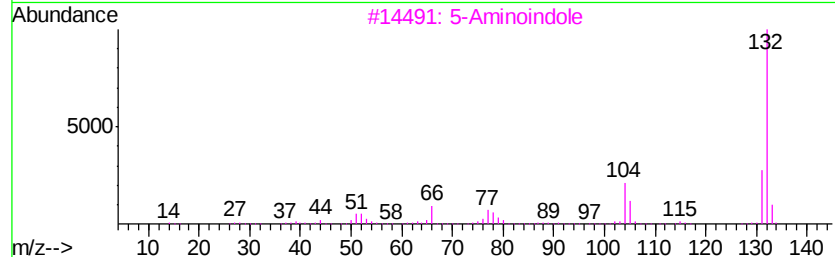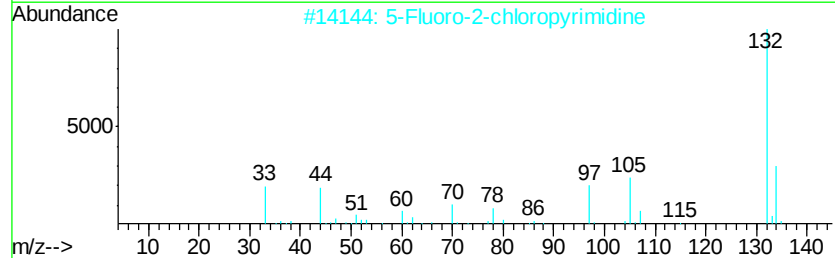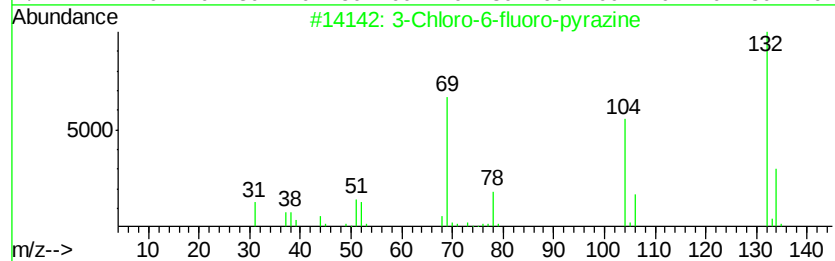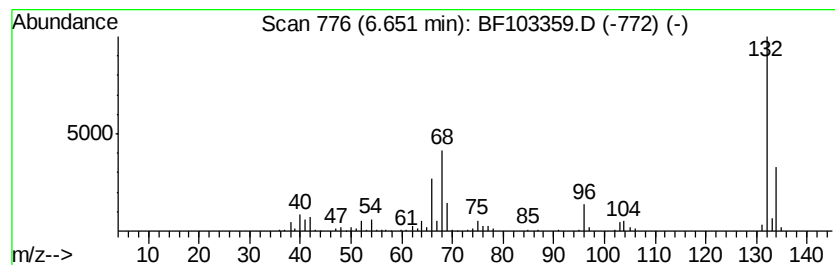

Data Path : Z:\HPCHEM1\BNA_F\Data\BF030218\
Data File : BF103359.D
Acq On : 2 Mar 2018 11:58
Operator : SJ/JU
Sample : PB106993BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB106993BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.65	6.65	12.6	ng	505066	1	6.87	802062	20.0