


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030218\
Data File : BF103354.D
Acq On : 2 Mar 2018 9:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 02 13:28:09 2018

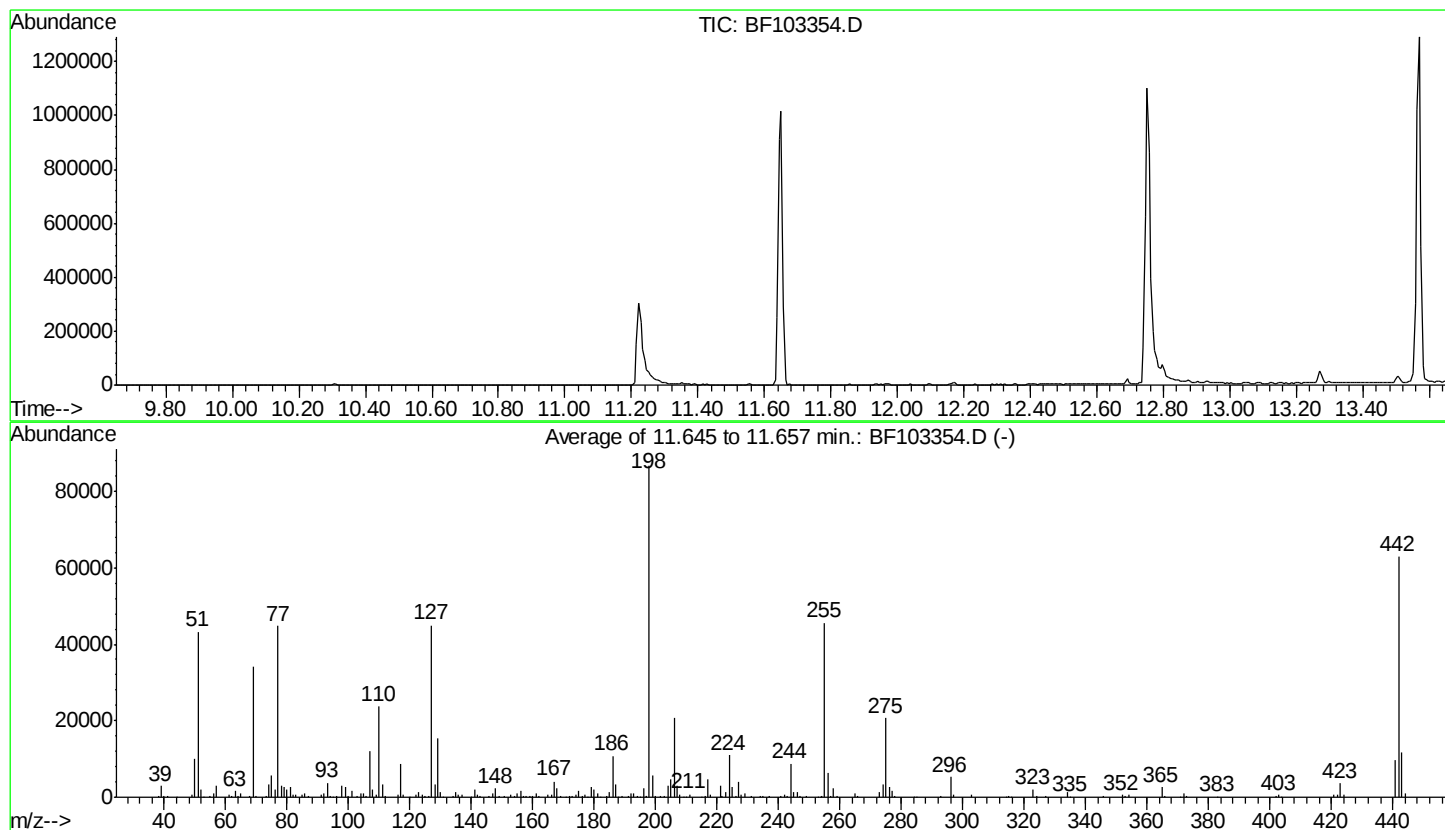

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	43266	PASS
68	69	0.00	2	1.4	493	PASS
69	198	0.00	100	39.3	34055	PASS
70	69	0.00	2	0.7	248	PASS
127	198	10	80	51.9	44988	PASS
197	198	0.00	2	0.4	389	PASS
198	198	100	100	100.0	86725	PASS
199	198	5	9	6.7	5820	PASS
275	198	10	60	23.9	20723	PASS
365	198	1	100	3.0	2612	PASS
441	443	0.01	100	84.2	9870	PASS
442	198	50	100	72.5	62914	PASS
443	442	15	24	18.6	11727	PASS