


Data Path : Z:\HPCHEM1\BNA F\Data\BF030218\
 Data File : BF103365.D
 Acq On : 2 Mar 2018 15:12
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 02 13:28:09 2018

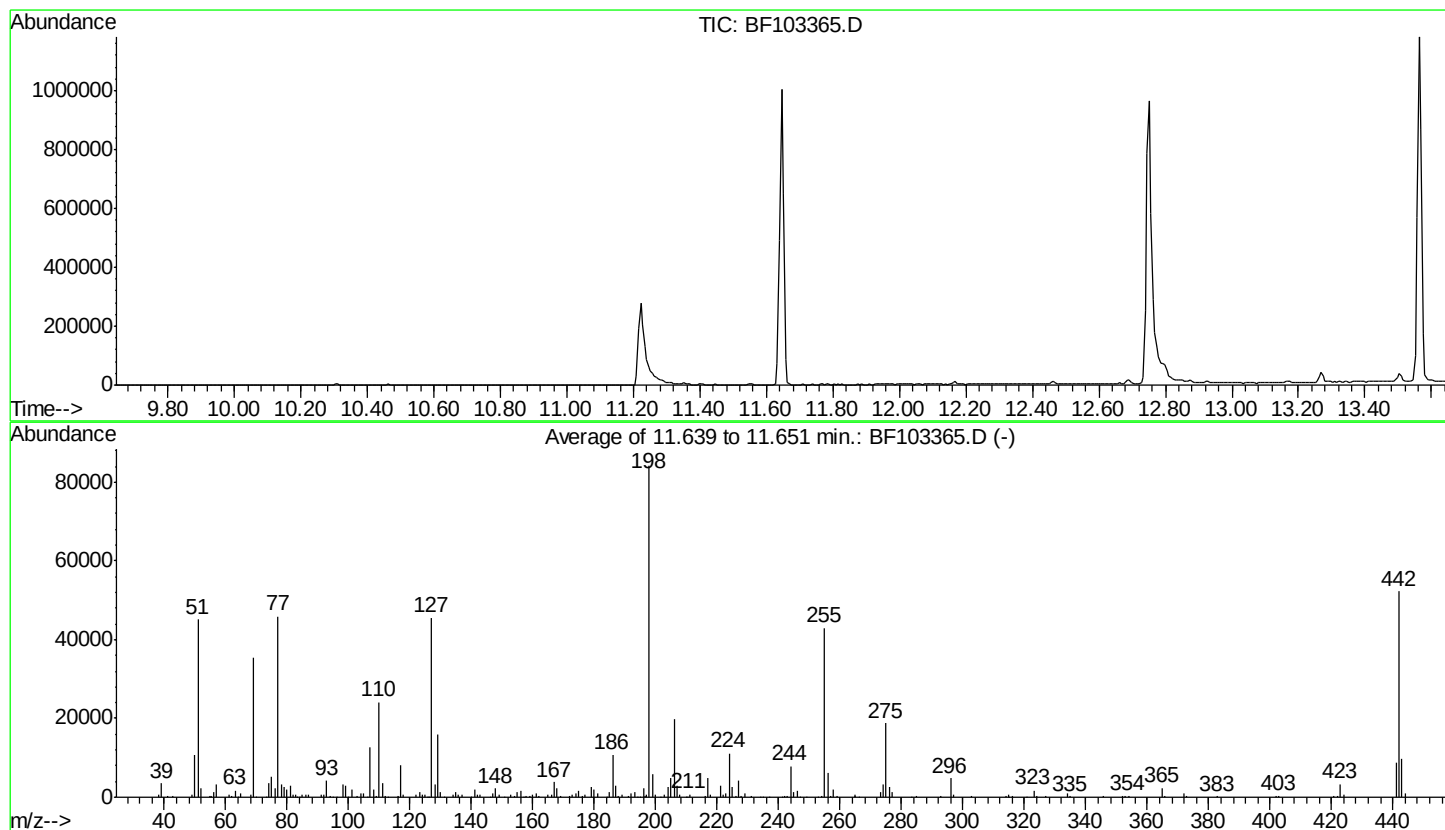

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	45066	PASS
68	69	0.00	2	1.8	621	PASS
69	198	0.00	100	41.9	35285	PASS
70	69	0.00	2	0.3	114	PASS
127	198	10	80	54.1	45514	PASS
197	198	0.00	2	0.6	538	PASS
198	198	100	100	100.0	84186	PASS
199	198	5	9	6.8	5734	PASS
275	198	10	60	22.4	18832	PASS
365	198	1	100	2.8	2329	PASS
441	443	0.01	100	89.4	8749	PASS
442	198	50	100	62.0	52183	PASS
443	442	15	24	18.8	9791	PASS