


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030218\
 Data File : BF103392.D
 Acq On : 3 Mar 2018 4:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 02 13:28:09 2018

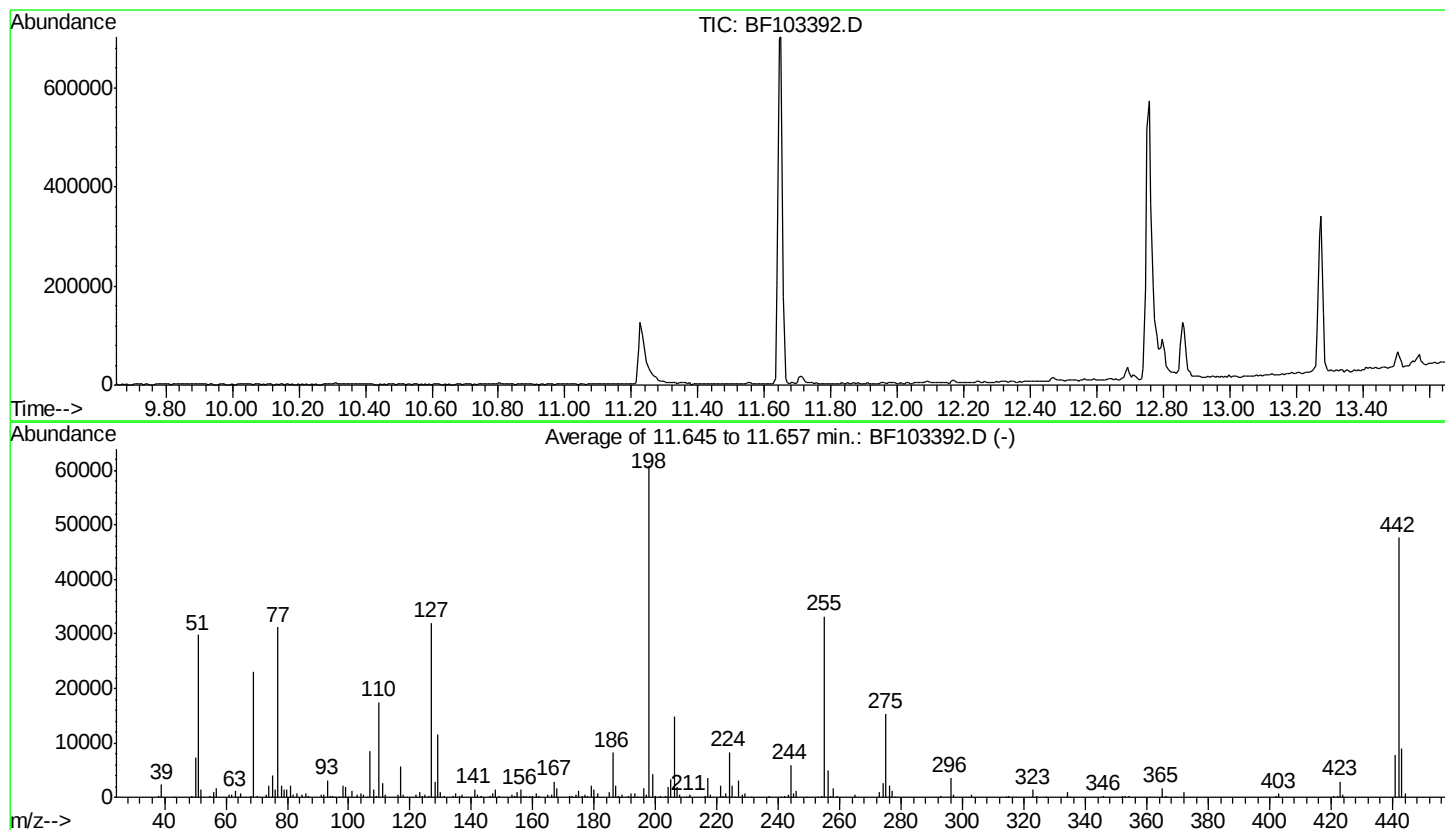

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	29819	PASS
68	69	0.00	2	1.3	300	PASS
69	198	0.00	100	37.8	23046	PASS
70	69	0.00	2	0.6	129	PASS
127	198	10	80	52.7	32084	PASS
197	198	0.00	2	0.8	471	PASS
198	198	100	100	100.0	60936	PASS
199	198	5	9	7.0	4255	PASS
275	198	10	60	25.3	15391	PASS
365	198	1	100	2.8	1684	PASS
441	443	0.01	100	88.7	7850	PASS
442	198	50	100	78.2	47682	PASS
443	442	15	24	18.6	8848	PASS