

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030222\
 Data File : BF127147.D
 Acq On : 02 Mar 2022 15:12
 Operator : CG\JU
 Sample : N1725-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-01

Quant Time: Mar 03 00:56:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 01 23:57:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.886	152	90950	20.000	ng	0.00
21) Naphthalene-d8	8.175	136	365871	20.000	ng	# 0.00
39) Acenaphthene-d10	9.933	164	188330	20.000	ng	0.00
64) Phenanthrene-d10	11.422	188	329047	20.000	ng	# 0.00
76) Chrysene-d12	14.068	240	151133	20.000	ng	# 0.00
86) Perylene-d12	15.562	264	162790	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	315499	53.615	ng	0.00
7) Phenol-d6	6.516	99	287654	36.227	ng	0.00
23) Nitrobenzene-d5	7.457	82	666926	82.278	ng	0.00
42) 2,4,6-Tribromophenol	10.727	330	211942	97.743	ng	0.00
45) 2-Fluorobiphenyl	9.251	172	1099255	85.928	ng	0.00
79) Terphenyl-d14	13.010	244	999150	97.185	ng	0.00
Target Compounds						
10) Phenol	6.528	94	18343	2.286	ng	Qvalue 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030222\
Data File : BF127147.D
Acq On : 02 Mar 2022 15:12
Operator : CG\JU
Sample : N1725-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-01

Quant Time: Mar 03 00:56:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 01 23:57:09 2022
Response via : Initial Calibration




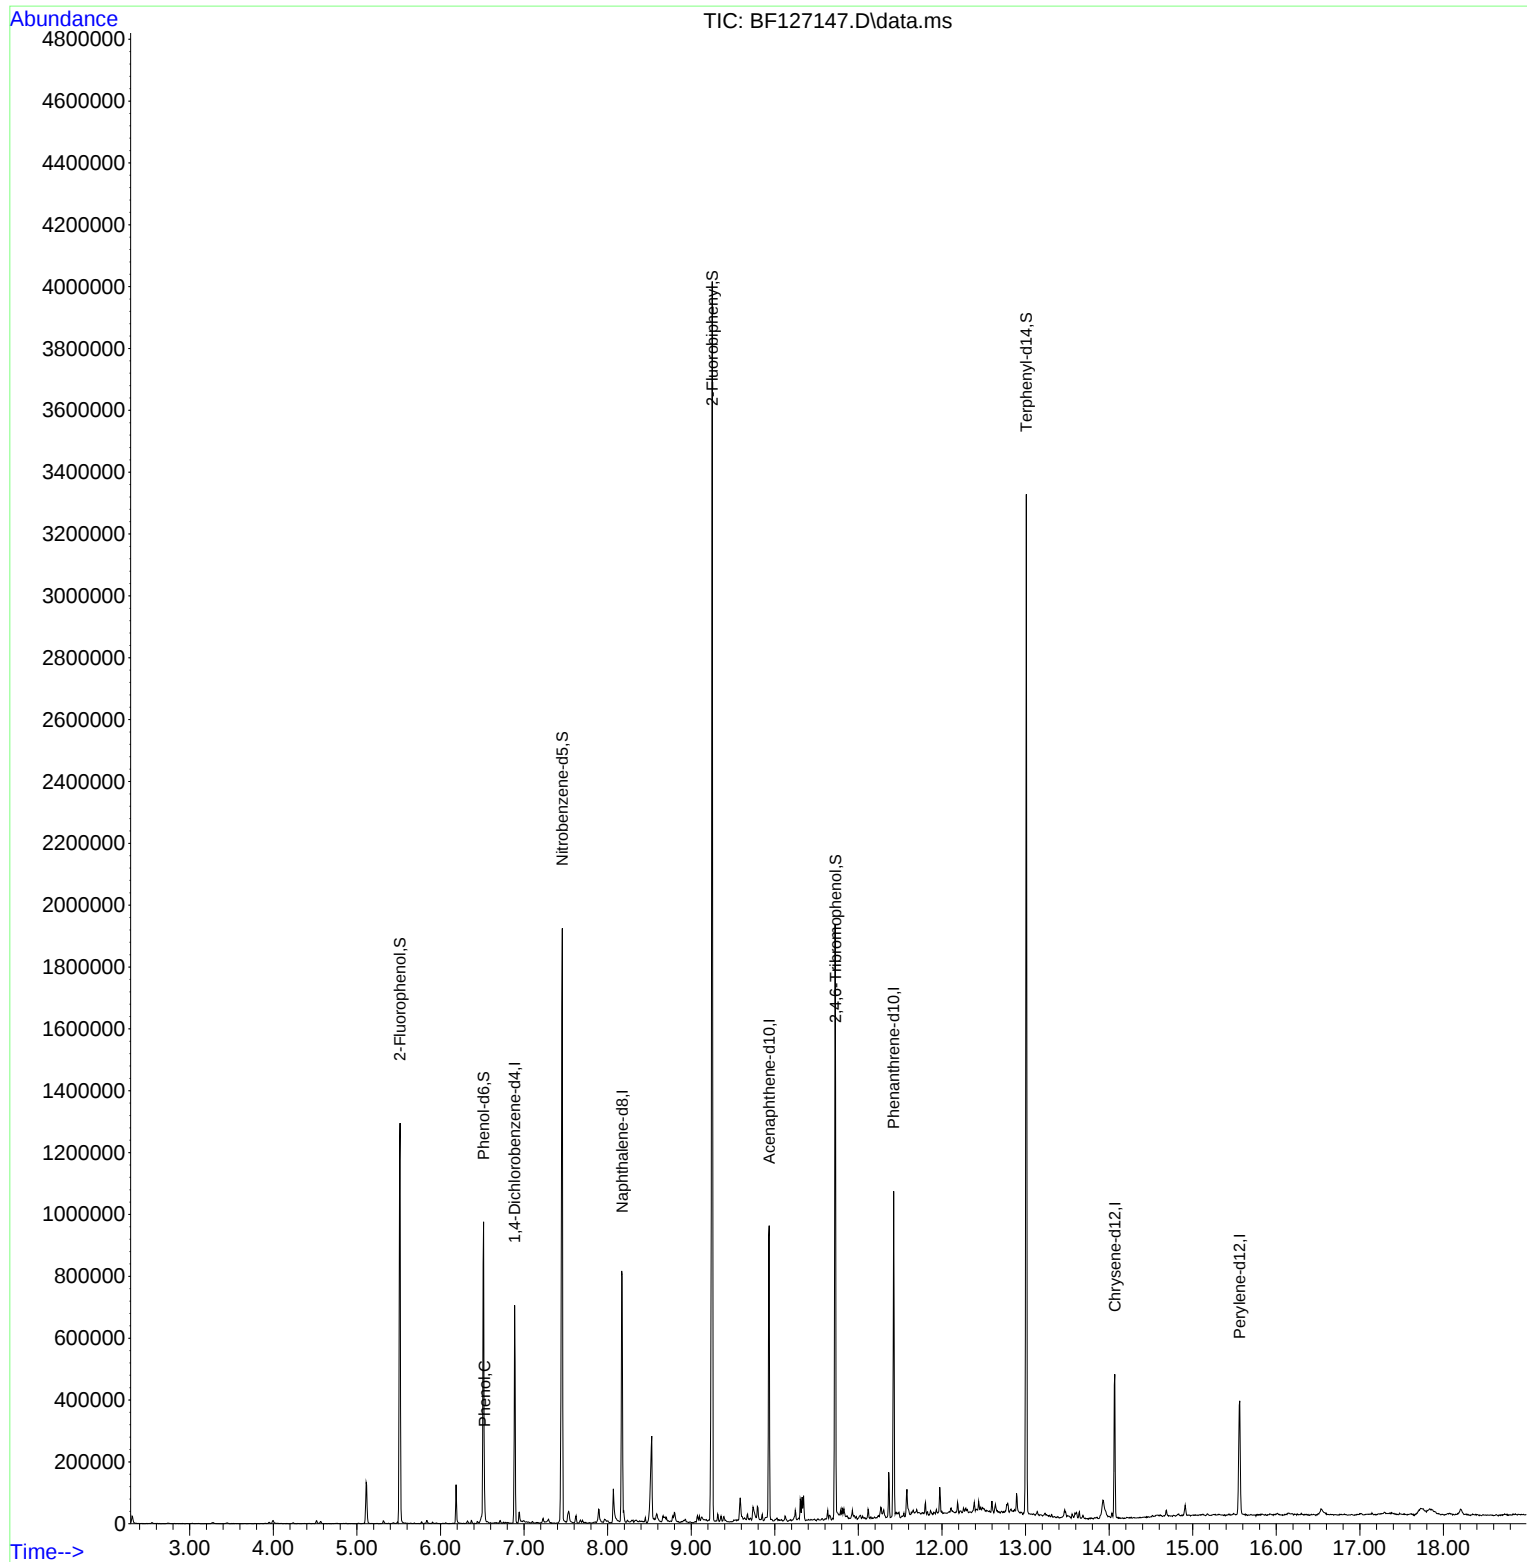




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.886 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF127147.D
Acq: 02 Mar 2022 15:12




Instrument :
BNA_F
ClientSampleId :
MW-01


Tgt Ion:152 Resp: 90950
Ion Ratio Lower Upper
152 100
150 153.8 128.1 192.1
115 69.1 56.7 85.1

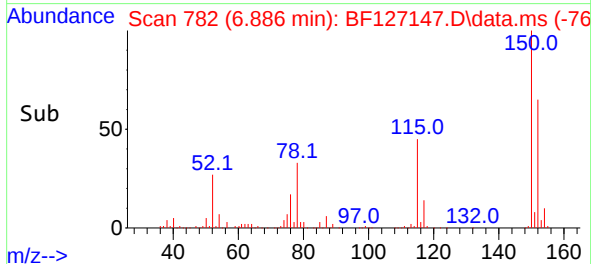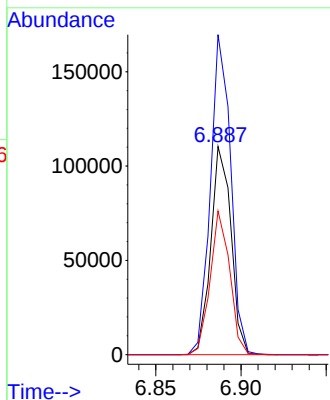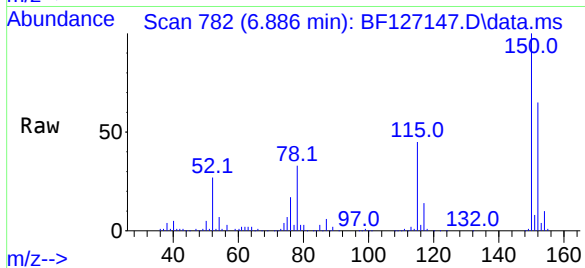

#5
2-Fluorophenol
Concen: 53.615 ng
RT: 5.516 min Scan# 549
Delta R.T. 0.006 min
Lab File: BF127147.D
Acq: 02 Mar 2022 15:12

Tgt Ion:112 Resp: 315499
Ion Ratio Lower Upper
112 100
64 65.3 49.5 74.3
63 34.4 23.9 35.9


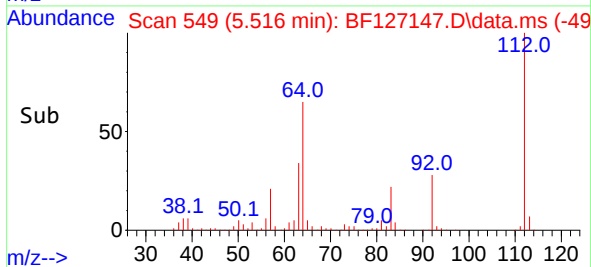
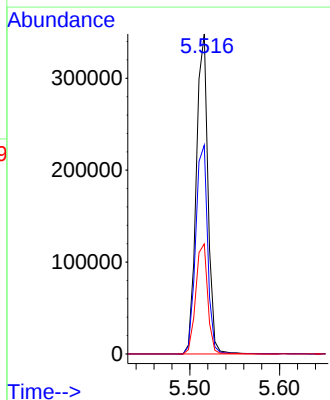
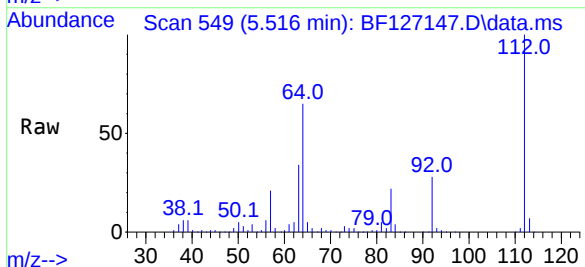




#7
Phenol-d6
Concen: 36.227 ng
RT: 6.516 min Scan# 719
Delta R.T. -0.006 min
Lab File: BF127147.D
Acq: 02 Mar 2022 15:12




Instrument :
BNA_F
ClientSampleId :
MW-01


Tgt Ion: 99 Resp: 287654
Ion Ratio Lower Upper
99 100
42 18.7 14.2 21.4
71 39.0 24.3 36.5#

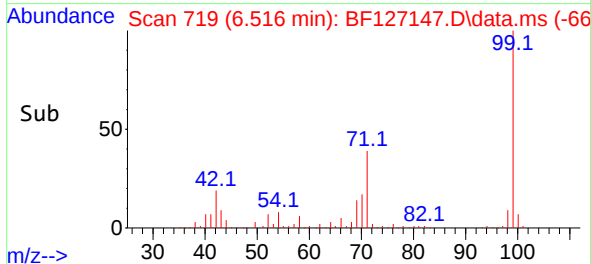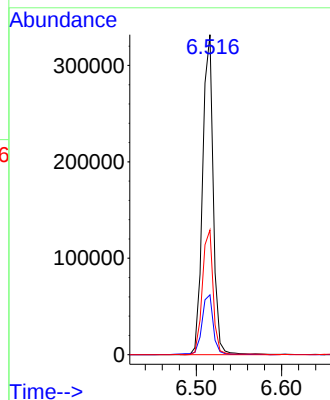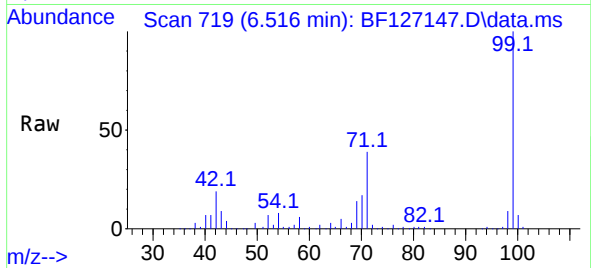

#10
Phenol
Concen: 2.286 ng
RT: 6.528 min Scan# 721
Delta R.T. -0.012 min
Lab File: BF127147.D
Acq: 02 Mar 2022 15:12

Tgt Ion: 94 Resp: 18343
Ion Ratio Lower Upper
94 100
65 33.1 7.2 47.2
66 48.7 14.5 54.5


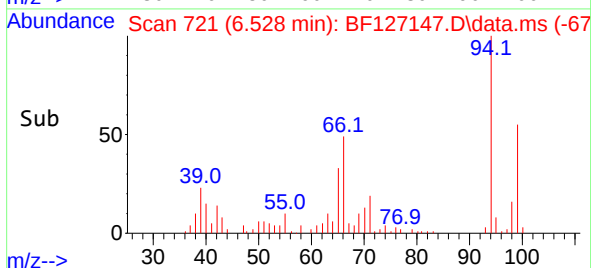
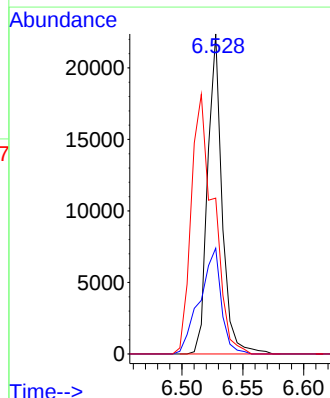
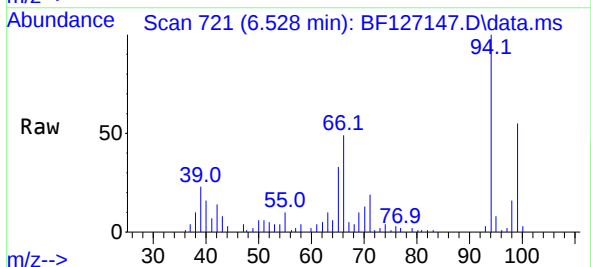




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.175 min Scan# 10
Delta R.T. -0.000 min
Lab File: BF127147.D
Acq: 02 Mar 2022 15:12




Instrument :
BNA_F
ClientSampleId :
MW-01


Tgt Ion:136 Resp: 365871
Ion Ratio Lower Upper
136 100
137 10.4 8.6 13.0
54 7.6 7.8 11.6#
68 4.6 6.3 9.5#

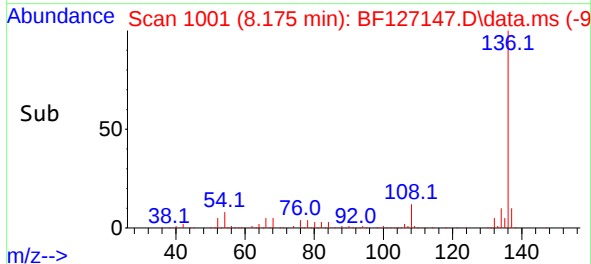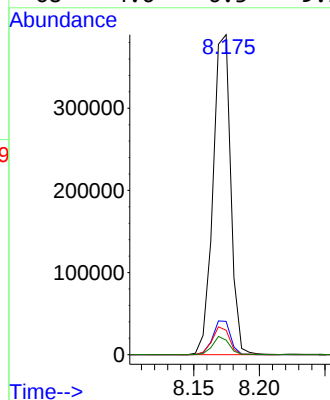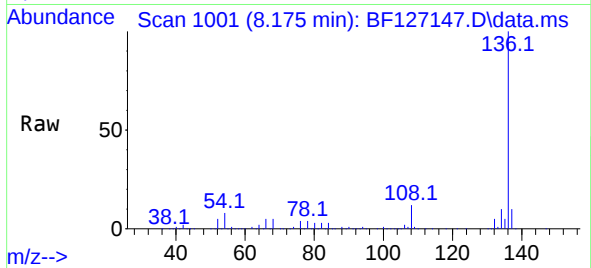

#23
Nitrobenzene-d5
Concen: 82.278 ng
RT: 7.457 min Scan# 879
Delta R.T. -0.006 min
Lab File: BF127147.D
Acq: 02 Mar 2022 15:12

Tgt Ion: 82 Resp: 666926
Ion Ratio Lower Upper
82 100
128 41.0 32.7 49.1
54 51.4 41.7 62.5

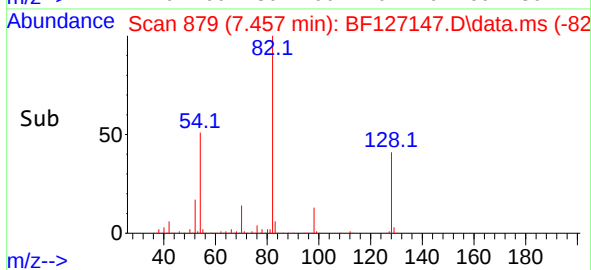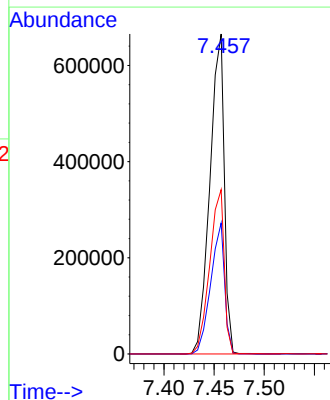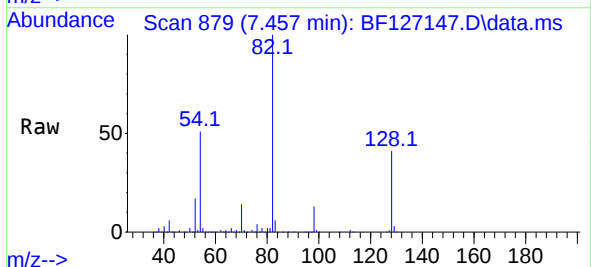



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.933 min Scan# 11

Delta R.T. -0.006 min

Lab File: BF127147.D

Acq: 02 Mar 2022 15:12

Instrument :

BNA_F

ClientSampleId :

MW-01





Tgt Ion:164 Resp: 188330

Ion Ratio Lower Upper

164 100

162 101.8 81.4 122.0

160 46.5 36.6 54.8

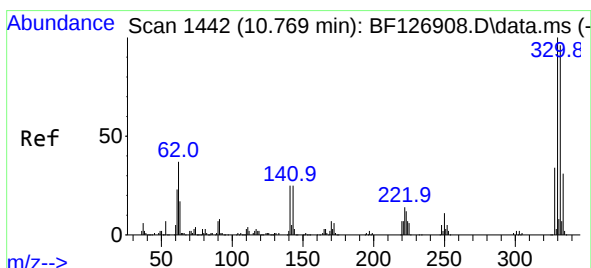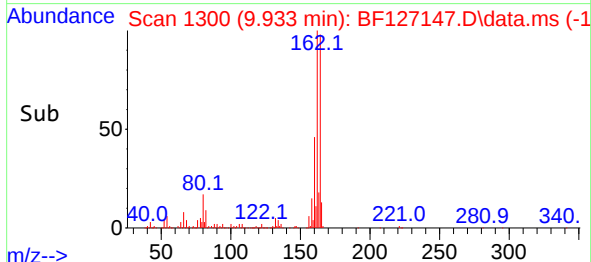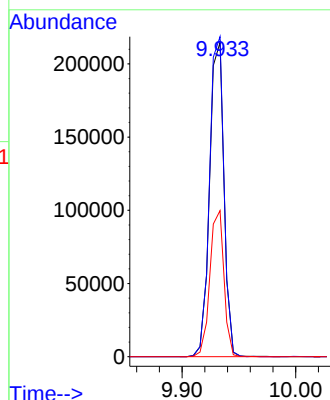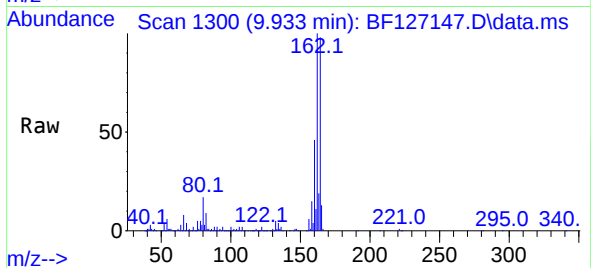

#42

2,4,6-Tribromophenol

Concen: 97.743 ng

RT: 10.727 min Scan# 1435

Delta R.T. -0.000 min

Lab File: BF127147.D

Acq: 02 Mar 2022 15:12




Tgt Ion:330 Resp: 211942


Ion Ratio Lower Upper

330 100

332 98.2 76.0 114.0

141 36.1 30.1 45.1

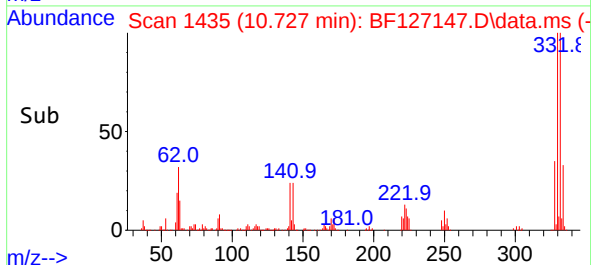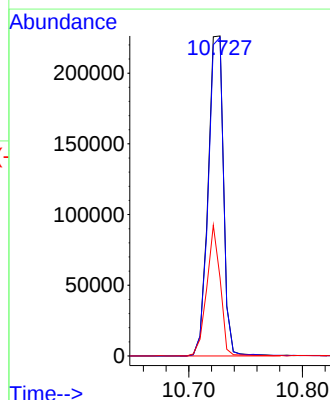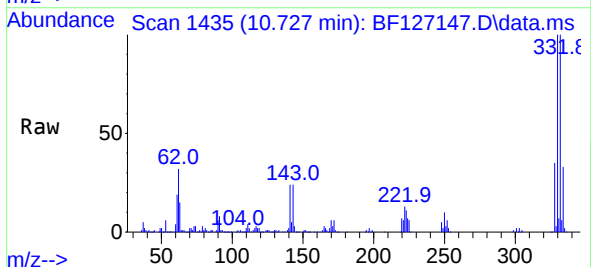

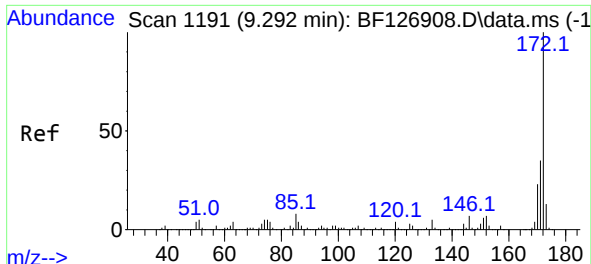

#45

2-Fluorobiphenyl

Concen: 85.928 ng

RT: 9.251 min Scan# 1191

Delta R.T. -0.000 min

Lab File: BF127147.D

Acq: 02 Mar 2022 15:12

Instrument :

BNA_F

ClientSampleId :

MW-01





Tgt Ion:172 Resp: 1099255

Ion Ratio Lower Upper

172 100

171 35.1 28.3 42.5

170 23.7 19.0 28.6

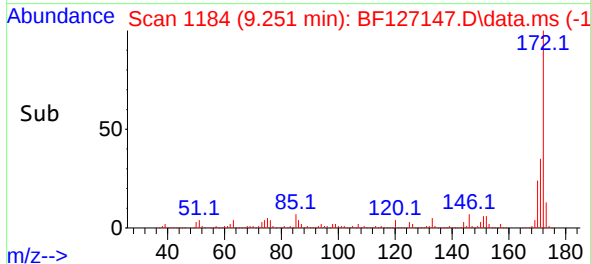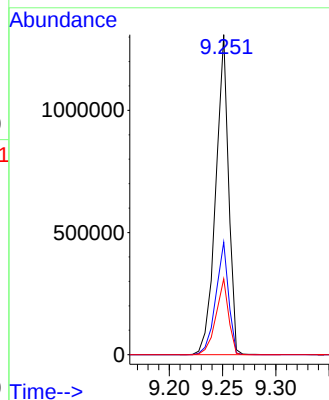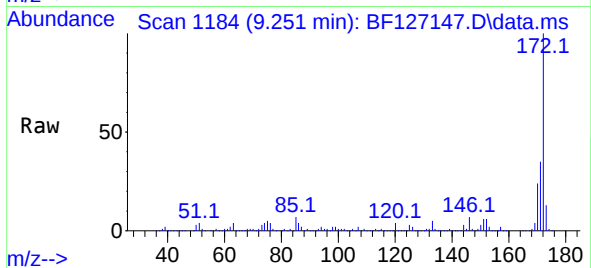

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.422 min Scan# 1553

Delta R.T. -0.006 min

Lab File: BF127147.D

Acq: 02 Mar 2022 15:12




Tgt Ion:188 Resp: 329047


Ion Ratio Lower Upper

188 100

94 9.0 10.1 15.1#

80 10.3 11.8 17.6#


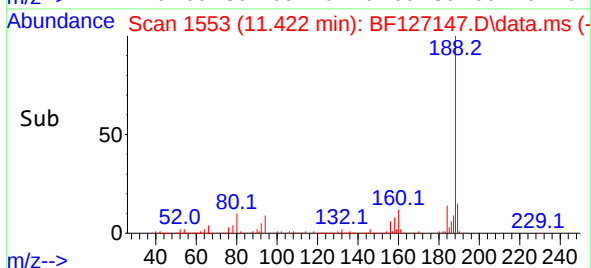
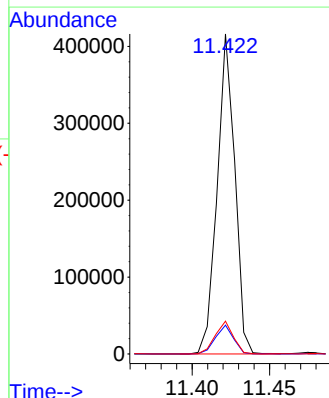
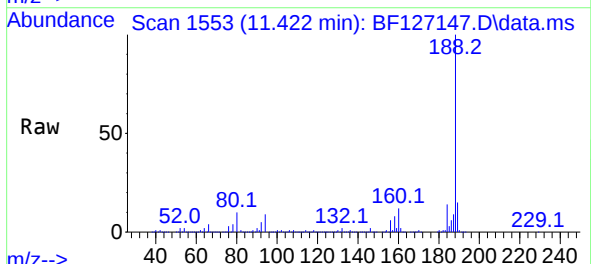




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.068 min Scan# 2010
Delta R.T. -0.006 min
Lab File: BF127147.D
Acq: 02 Mar 2022 15:12




Instrument :
BNA_F
ClientSampleId :
MW-01


Tgt Ion:240 Resp: 151133
Ion Ratio Lower Upper
240 100
120 10.2 14.4 21.6#
236 24.9 20.5 30.7

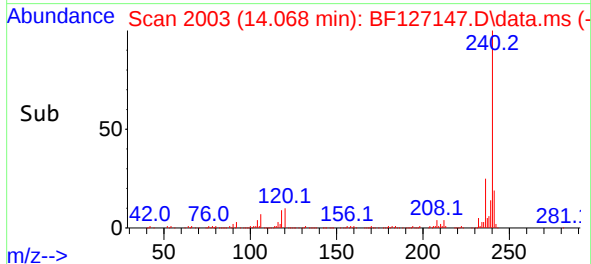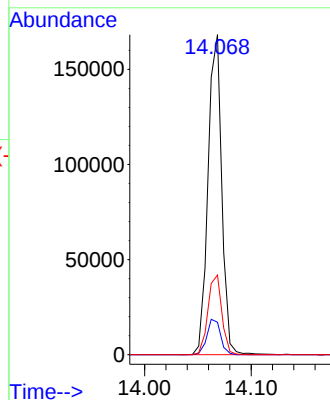

#79
Terphenyl-d14
Concen: 97.185 ng
RT: 13.010 min Scan# 1823
Delta R.T. -0.006 min
Lab File: BF127147.D
Acq: 02 Mar 2022 15:12

Tgt Ion:244 Resp: 999150
Ion Ratio Lower Upper
244 100
212 6.9 5.0 7.4
122 11.1 13.3 19.9#

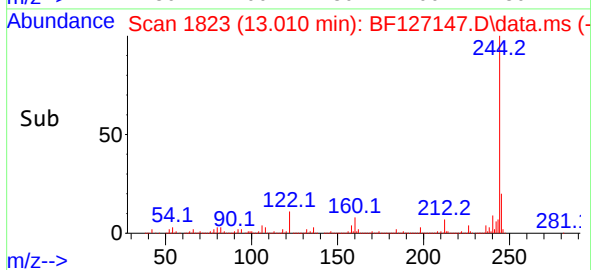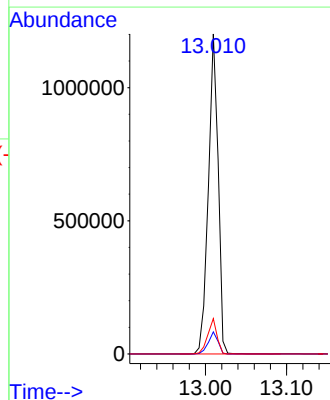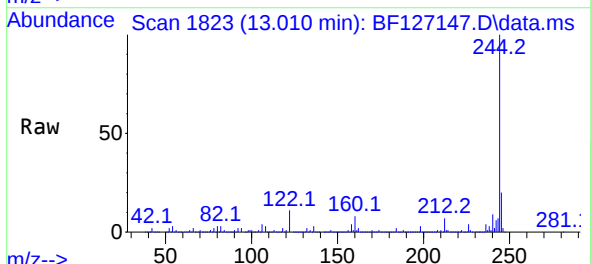

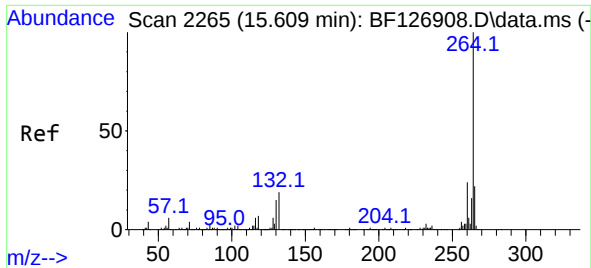

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.562 min Scan# 21
Delta R.T. -0.006 min
Lab File: BF127147.D
Acq: 02 Mar 2022 15:12

Instrument :
BNA_F
ClientSampleId :
MW-01

Tgt Ion:264 Resp: 162790

Ion	Ratio	Lower	Upper
264	100		
260	22.7	19.2	28.8
265	20.6	17.4	26.2

