

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030222\
 Data File : BF127148.D
 Acq On : 02 Mar 2022 15:41
 Operator : CG\JU
 Sample : N1725-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-02

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.110	477	480	486	rVB	39456	44215	1.18%	0.247%
2	5.510	544	548	551	rBV	1870744	1575259	41.90%	8.802%
3	6.516	715	719	732	rVB	1233729	1086131	28.89%	6.069%
4	6.886	779	782	786	rBV	648529	542477	14.43%	3.031%
5	7.457	873	879	882	rBV	2291531	2143632	57.02%	11.978%
6	8.069	980	983	996	rBV	40401	55522	1.48%	0.310%
7	8.175	996	1001	1004	rBV	837422	739407	19.67%	4.131%
8	8.510	1052	1058	1068	rBV	142704	185524	4.93%	1.037%
9	9.251	1178	1184	1187	rBV	4487880	3759658	100.00%	21.007%
10	9.927	1296	1299	1303	rBV	847775	776274	20.65%	4.337%
11	10.727	1430	1435	1438	rBV	2450305	2385906	63.46%	13.331%
12	11.363	1540	1543	1547	rVB	73939	60095	1.60%	0.336%
13	11.421	1549	1553	1556	rBV	983082	773426	20.57%	4.322%
14	11.580	1577	1580	1586	rBV	57924	67809	1.80%	0.379%
15	11.974	1644	1647	1653	rVB	55419	47771	1.27%	0.267%
16	13.010	1818	1823	1826	rBV	3124315	2763461	73.50%	15.441%
17	13.927	1976	1979	1986	rBV3	36609	65334	1.74%	0.365%
18	14.068	1999	2003	2006	rBV	399736	367490	9.77%	2.053%
19	15.562	2251	2257	2261	rBV	341390	457511	12.17%	2.556%




Sum of corrected areas: 17896902

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030222\
Data File : BF127148.D
Acq On : 02 Mar 2022 15:41
Operator : CG\JU
Sample : N1725-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

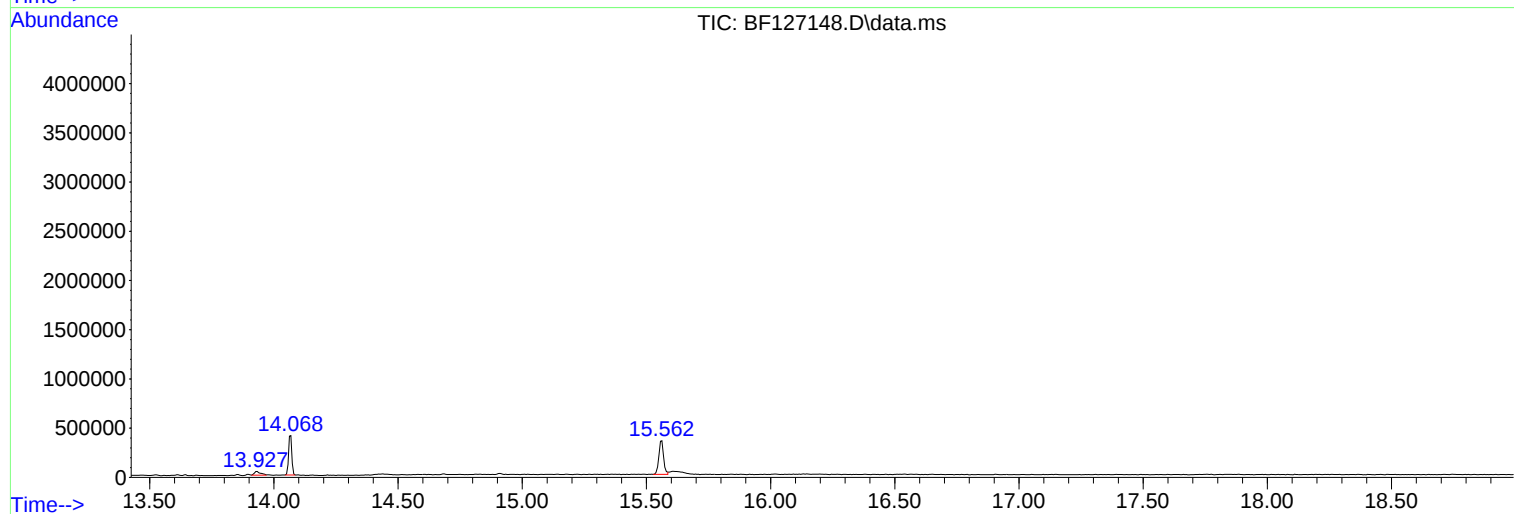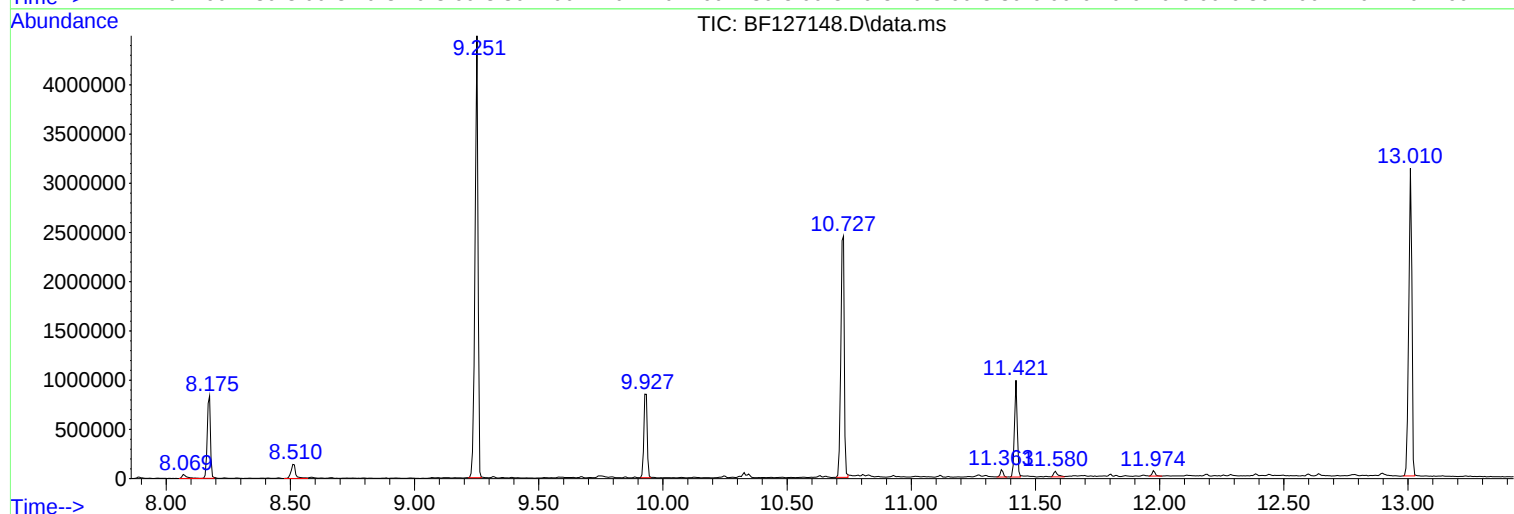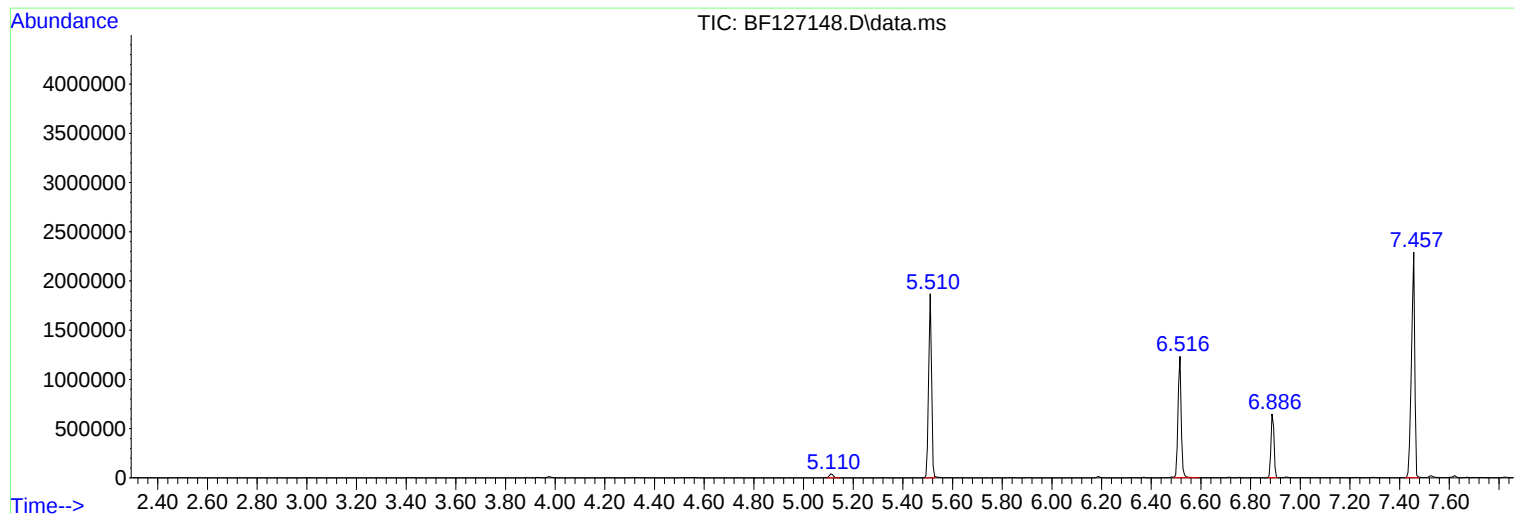

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030222\
Data File : BF127148.D
Acq On : 02 Mar 2022 15:41
Operator : CG\JU
Sample : N1725-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-02










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Octanoic acid, silver(1+) salt Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.510	5.02 ng	185524	Naphthalene-d8	8.175

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Octanoic acid, silver(1+) salt	250	C8H15AgO2	024927-67-1	53
2			Nonanoic acid	158	C9H18O2	000112-05-0	53
3			Octanoic acid	144	C8H16O2	000124-07-2	50
4			Hexanoic acid	116	C6H12O2	000142-62-1	49
5			Pentanoic acid, 3-methyl-	116	C6H12O2	000105-43-1	47

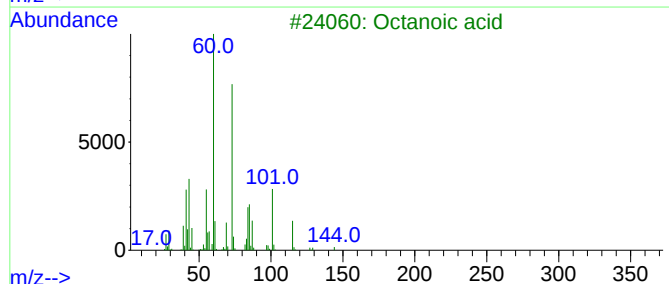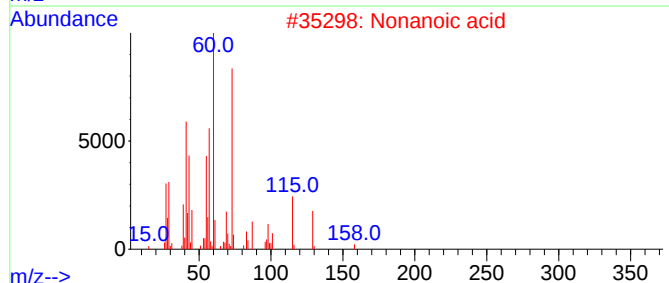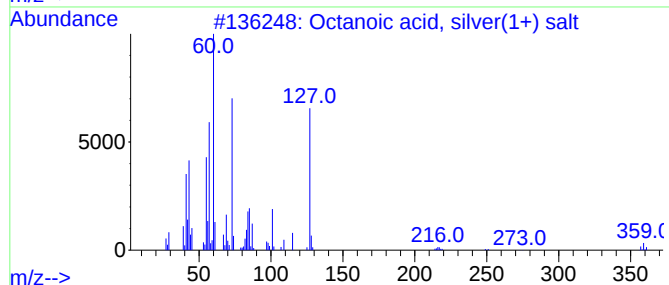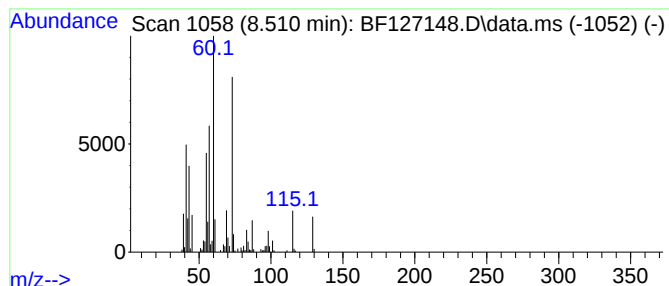

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030222\
Data File : BF127148.D
Acq On : 02 Mar 2022 15:41
Operator : CG\JU
Sample : N1725-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-02










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown13.927 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.927	3.56 ng	65334	Chrysene-d12	14.068

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			N-[(2-Phenyl-1,3-dioxolan-2-yl)m...	193	C10H11NO3	1000411-48-9	47
2			Benzoic acid, 2-(2-chlorophenoxy...	276	C15H13ClO3	1000368-25-9	47
3			Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	43
4			2-(2-(2-Methoxyethoxy)ethoxy)eth...	268	C14H20O5	1000366-99-1	38
5			Oxazolidine, 3-phenyl-	149	C9H11NO	020503-92-8	35

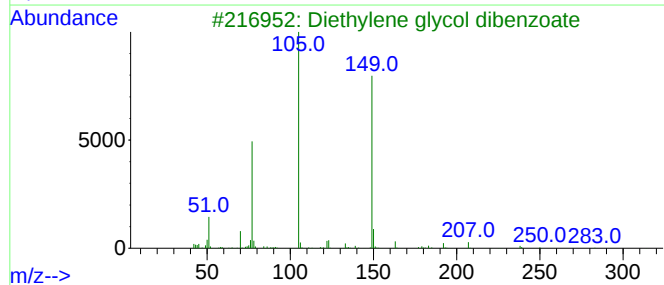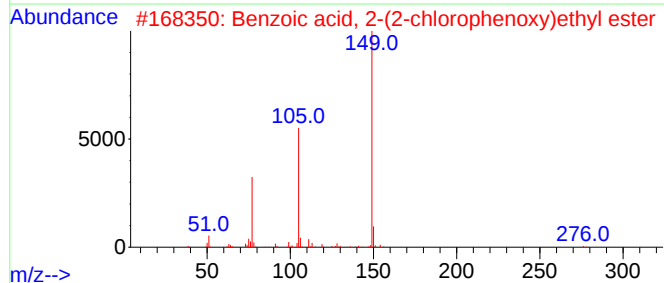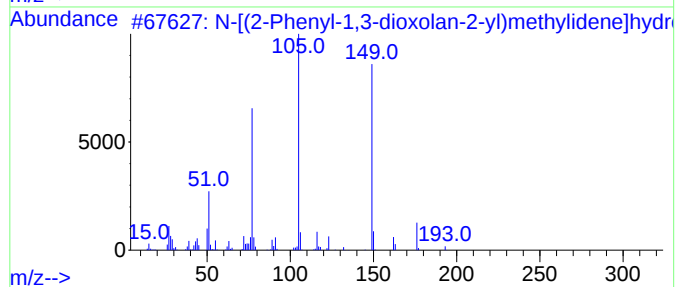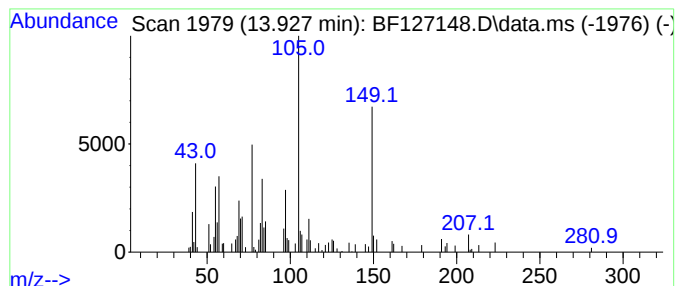

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030222\
Data File : BF127148.D
Acq On : 02 Mar 2022 15:41
Operator : CG\JU
Sample : N1725-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Octanoic acid, ...	8.510	5.0	ng	185524	2	8.175	739407	20.0
unknown13.927	13.927	3.6	ng	65334	5	14.068	367490	20.0