
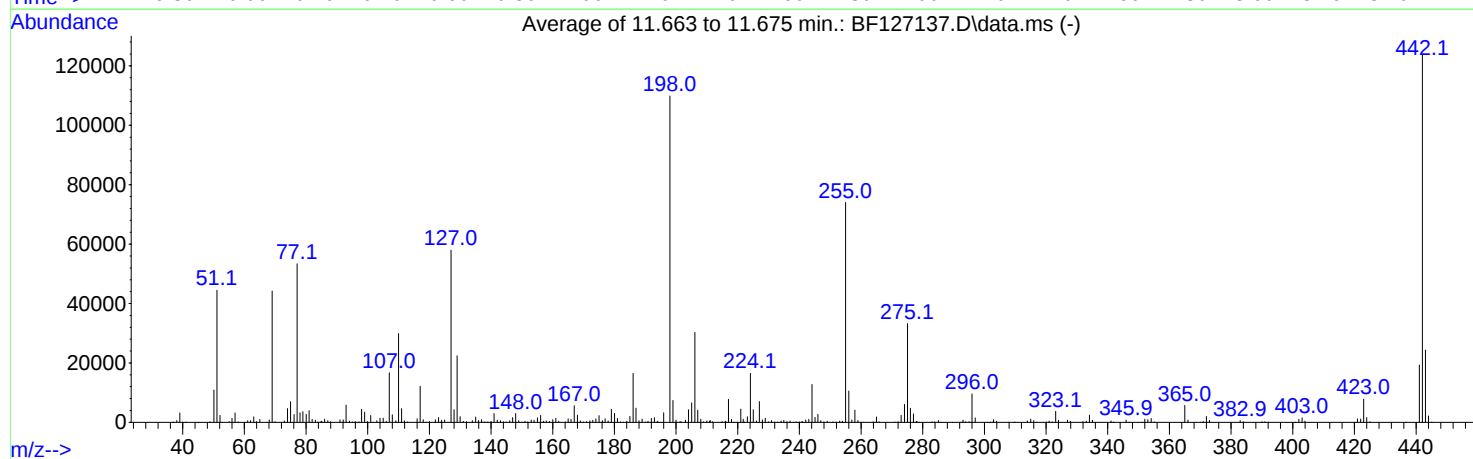


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030222\
 Data File : BF127137.D
 Acq On : 02 Mar 2022 10:18
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 01 23:57:09 2022

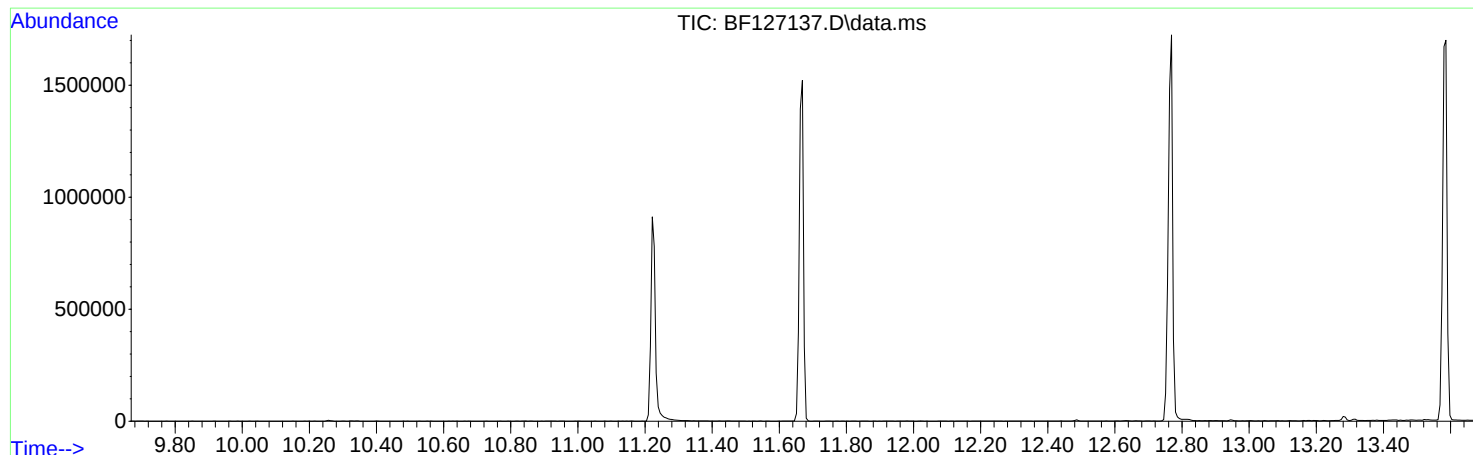




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	44511	PASS
68	69	0.00	2	1.9	827	PASS
69	198	0.00	100	40.3	44233	PASS
70	69	0.00	2	0.5	233	PASS
127	198	10	80	52.8	57967	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109867	PASS
199	198	5	9	6.7	7378	PASS
275	198	10	60	30.3	33276	PASS
365	198	1	100	5.2	5696	PASS
441	198	0.01	100	17.6	19287	PASS
442	442	50	100	100.0	123827	PASS
443	442	15	24	19.6	24325	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030222\
 Data File : BF127137.D
 Acq On : 02 Mar 2022 10:18
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 03 04:22:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 01 23:57:09 2022
 Response via : Initial Calibration

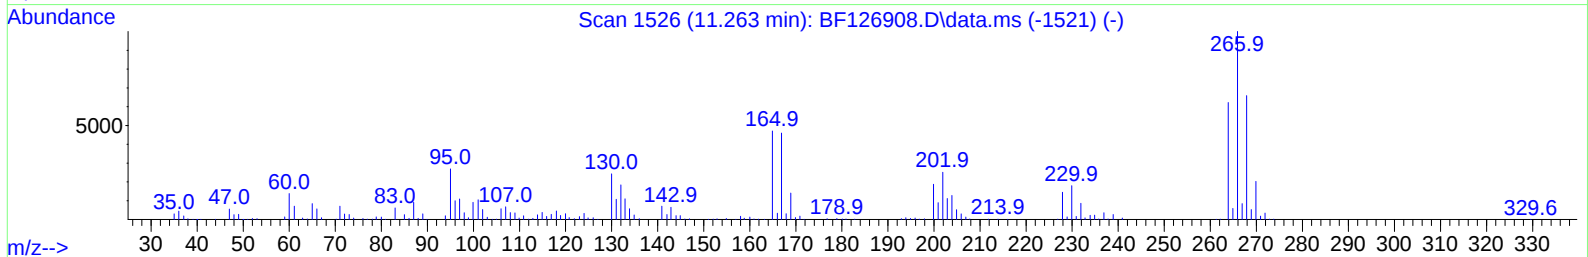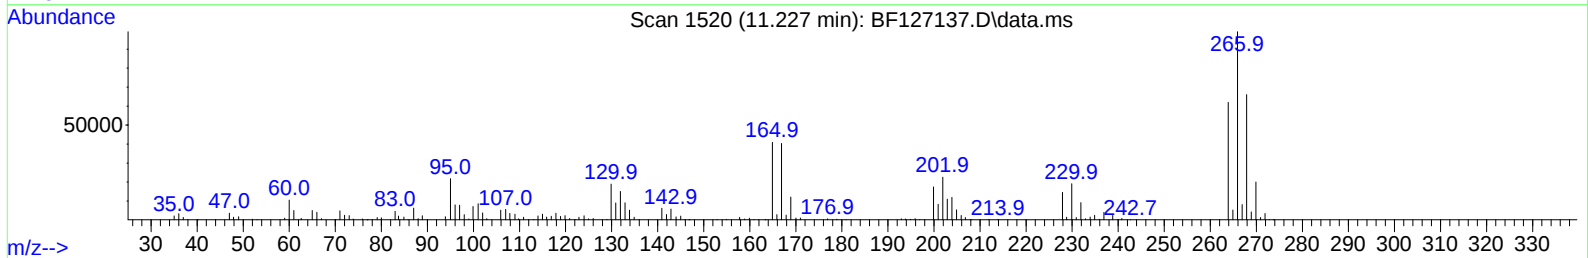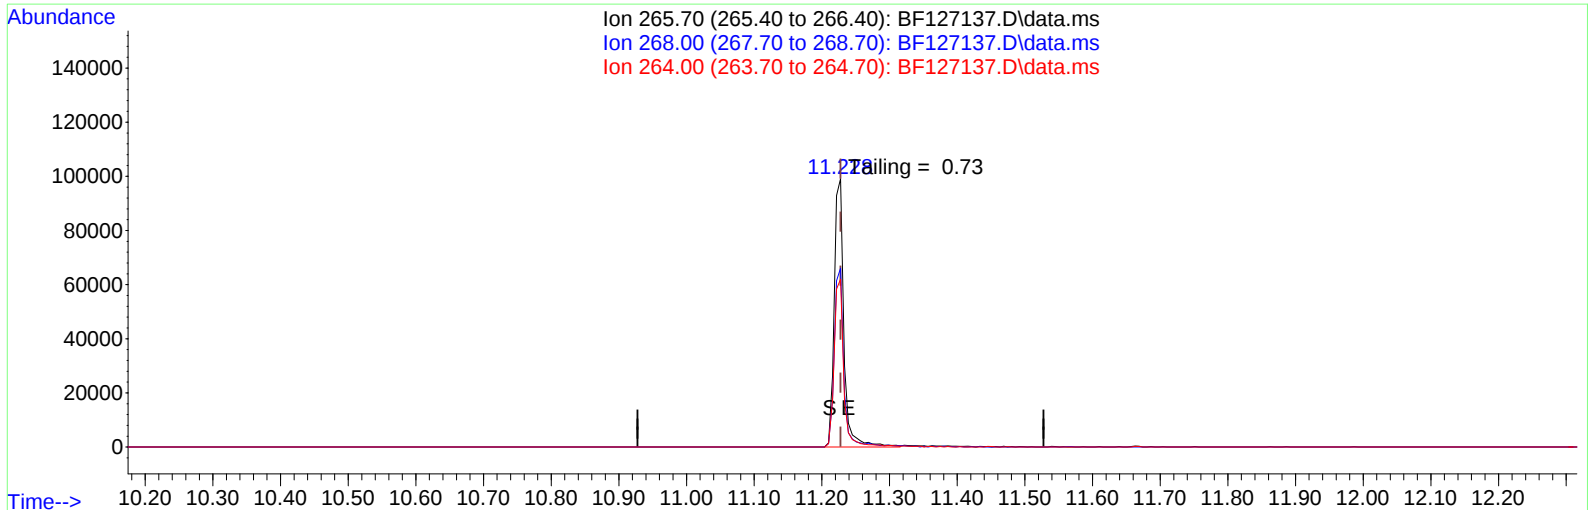

TIC: BF127137.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 22088.74 ng




response 98188

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.64
264.00	63.00	62.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030222\
Data File : BF127137.D
Acq On : 02 Mar 2022 10:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 03 04:22:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 01 23:57:09 2022
Response via : Initial Calibration

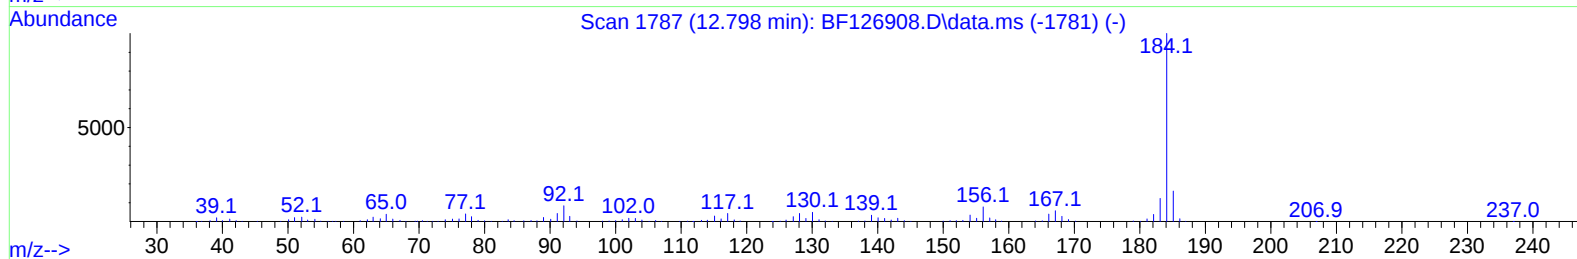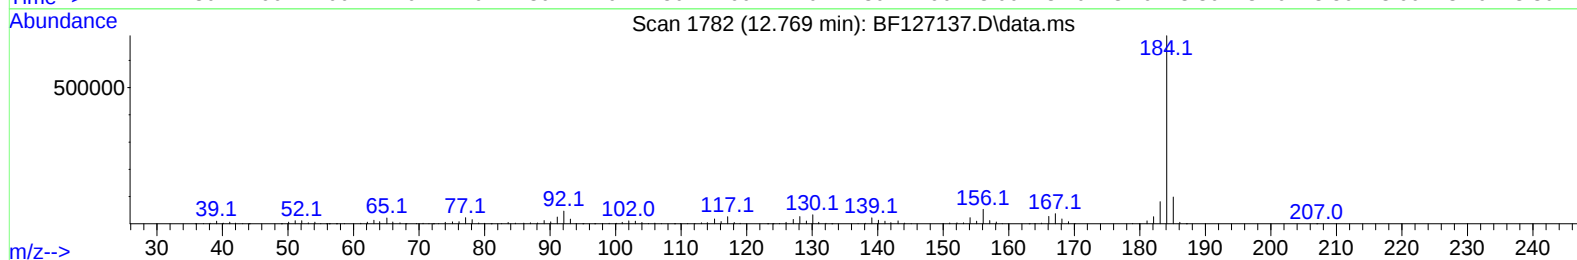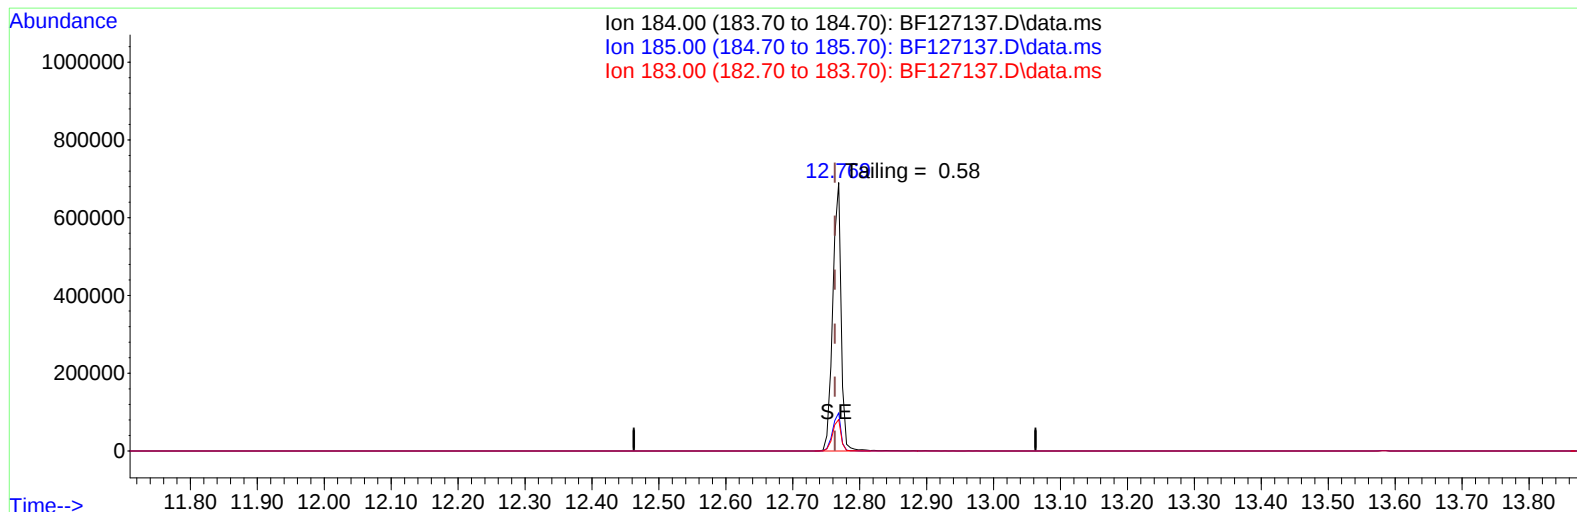

TIC: BF127137.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 0.00 ng

response 605743

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.27
183.00	10.20	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/2/2022	BNA_F	<u>BF127137.D</u>
Compound Name	Response	Retention Time
DDT	282694	13.586
DDD	4904	13.28
DDE	735	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5639	288333	1.96

Instrument :
BNA_F
ClientSampleId :
DFTPP