
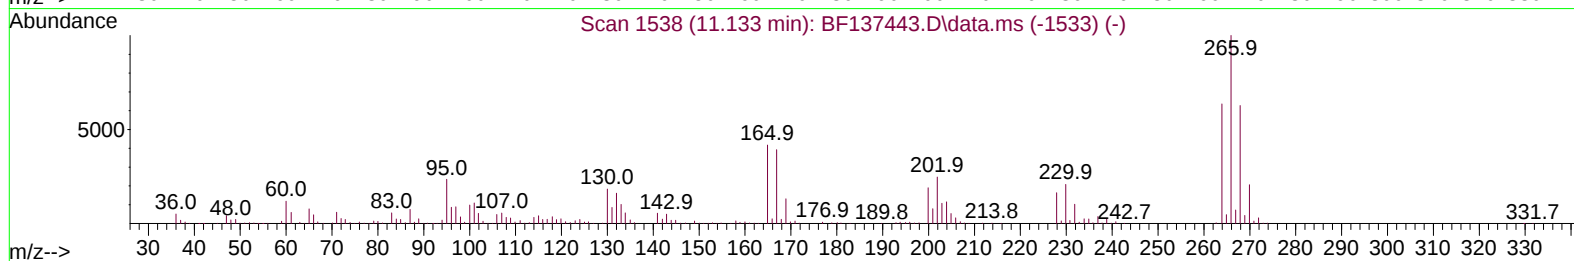
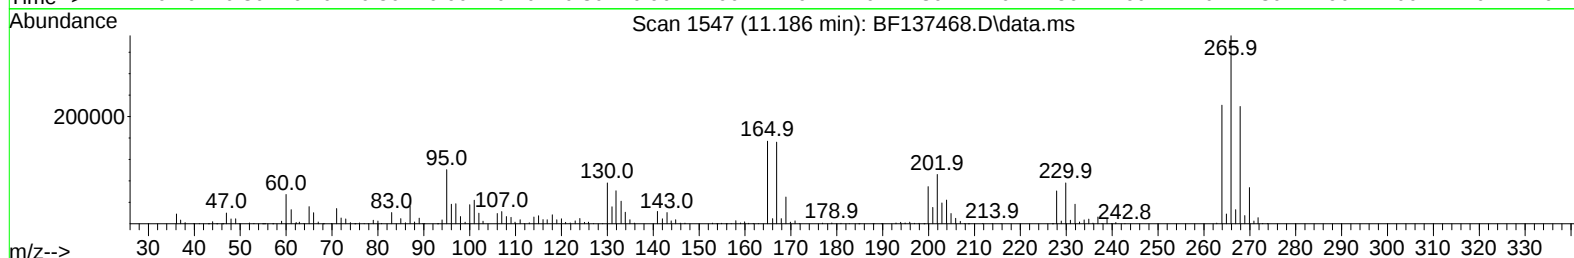


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030224\
Data File : BF137468.D
Acq On : 02 Mar 2024 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 00:47:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 00:26:53 2024
Response via : Initial Calibration

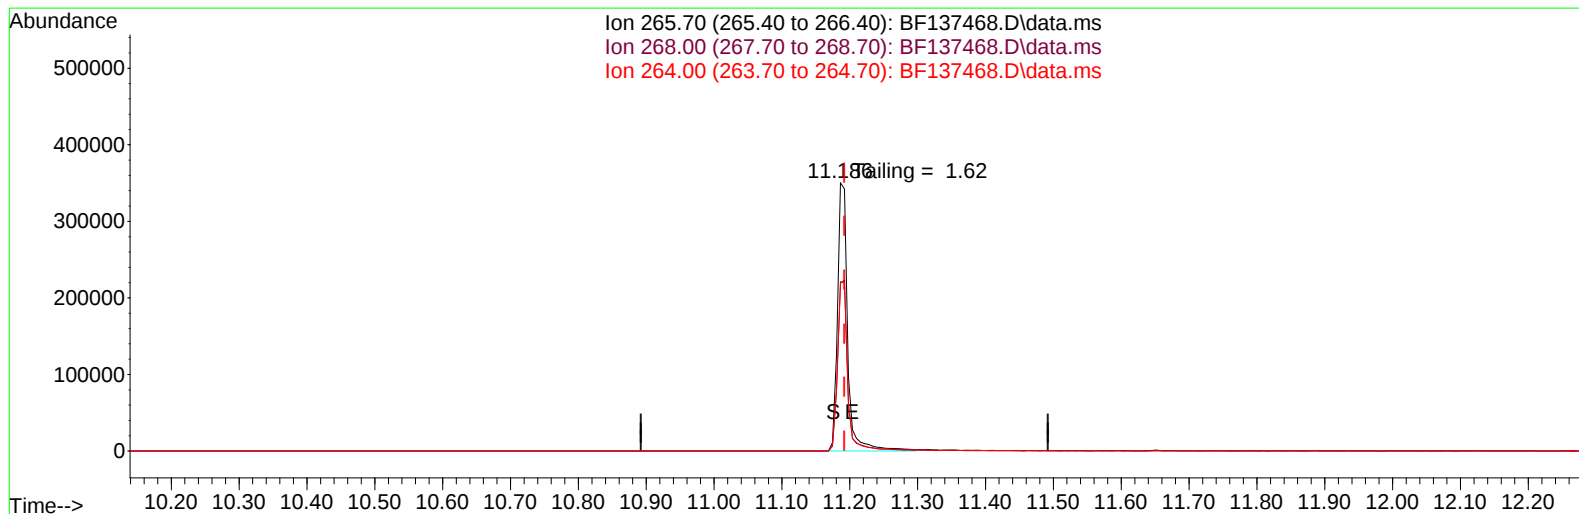

TIC: BF137468.D\data.ms

(70) Pentachlorophenol (C)




11.186min (-0.006) 297847.57 ng

response 364459

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.41
264.00	63.60	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030224\
Data File : BF137468.D
Acq On : 02 Mar 2024 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 00:47:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 00:26:53 2024
Response via : Initial Calibration

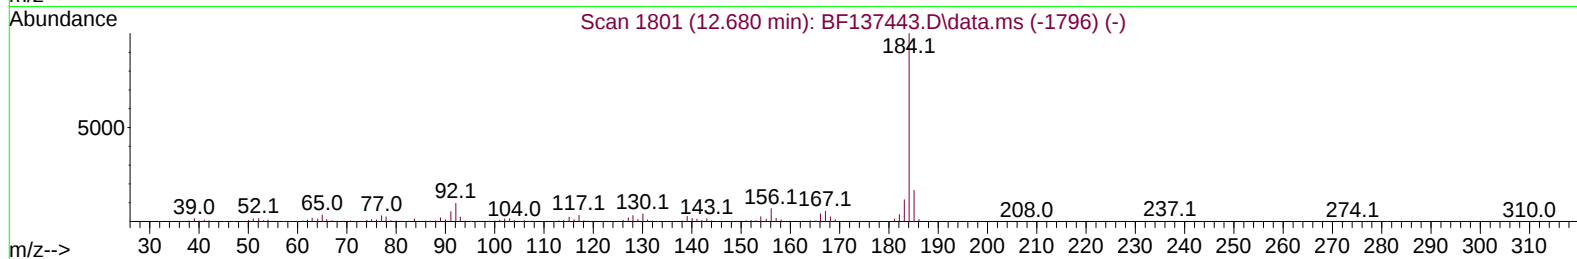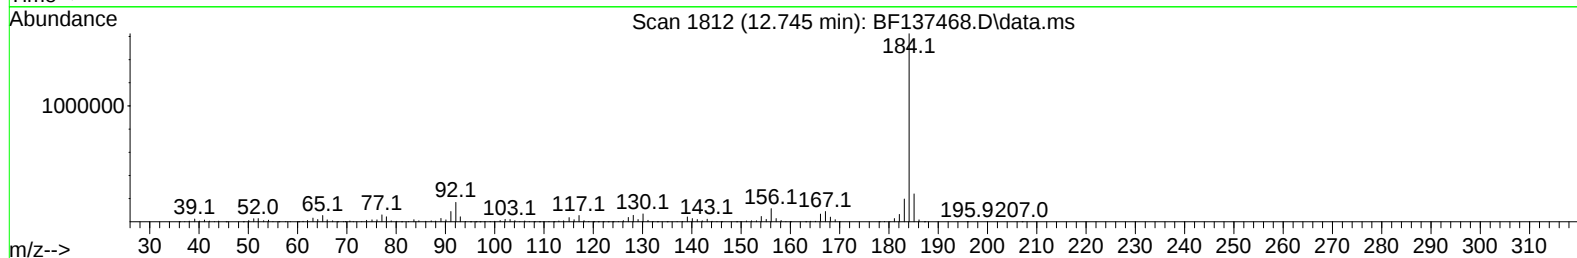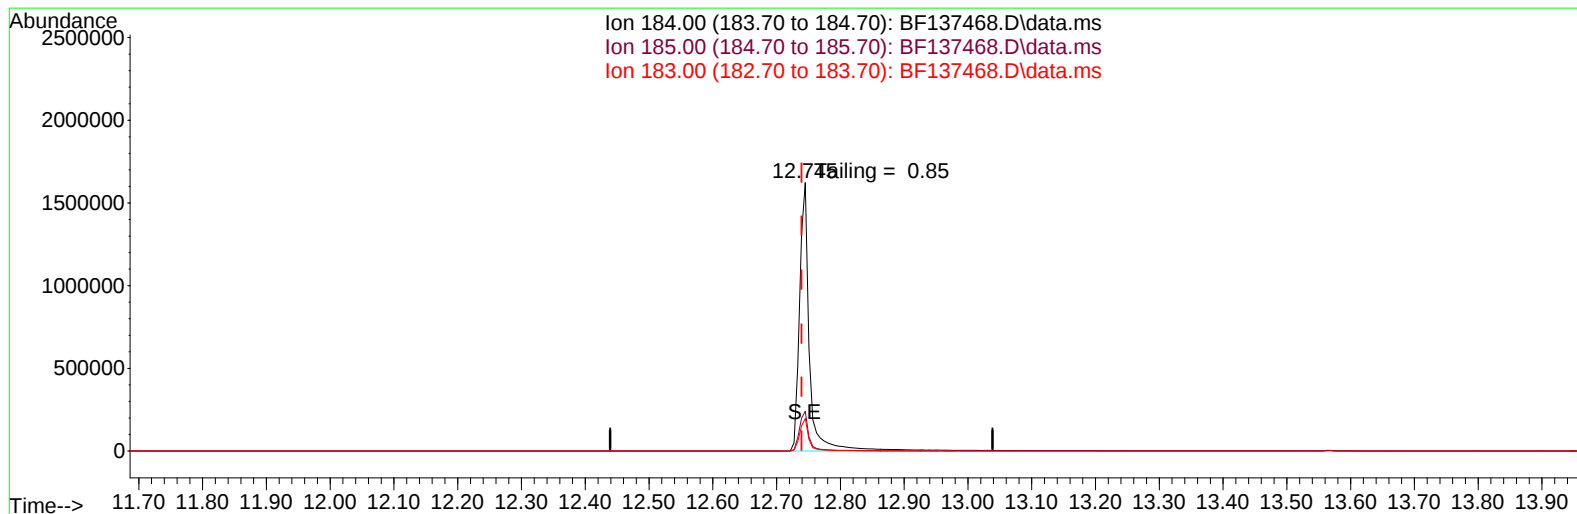

TIC: BF137468.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 6307.47 ng m

response 1770333

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.50	14.81
183.00	11.60	12.11
0.00	0.00	0.00