


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030224\
Data File : BF137468.D
Acq On : 02 Mar 2024 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 04 00:26:53 2024

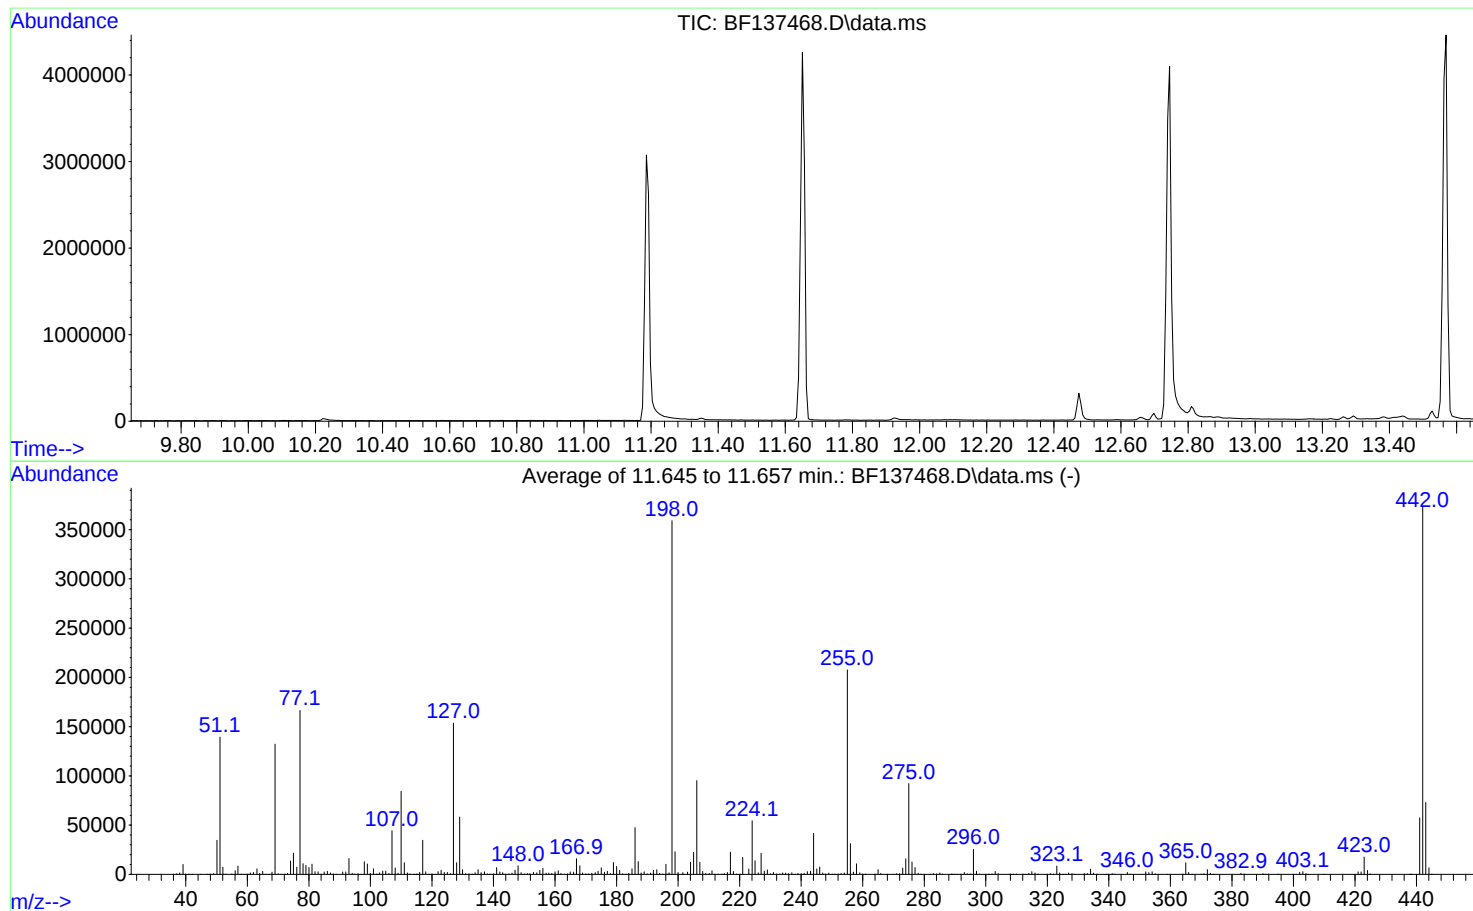




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	139341	PASS
68	69	0.00	2	1.7	2303	PASS
69	198	0.00	100	36.8	132184	PASS
70	69	0.00	2	0.6	742	PASS
127	198	10	80	42.8	153627	PASS
197	198	0.00	2	0.5	1631	PASS
198	198	100	100	100.0	359104	PASS
199	198	5	9	6.4	23005	PASS
275	198	10	60	25.7	92128	PASS
365	198	1	100	3.2	11633	PASS
441	198	0.01	100	16.0	57424	PASS
442	442	50	100	100.0	373525	PASS
443	442	15	24	19.5	72888	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030224\
Data File : BF137468.D
Acq On : 02 Mar 2024 12:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 04 00:47:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 00:26:53 2024
Response via : Initial Calibration

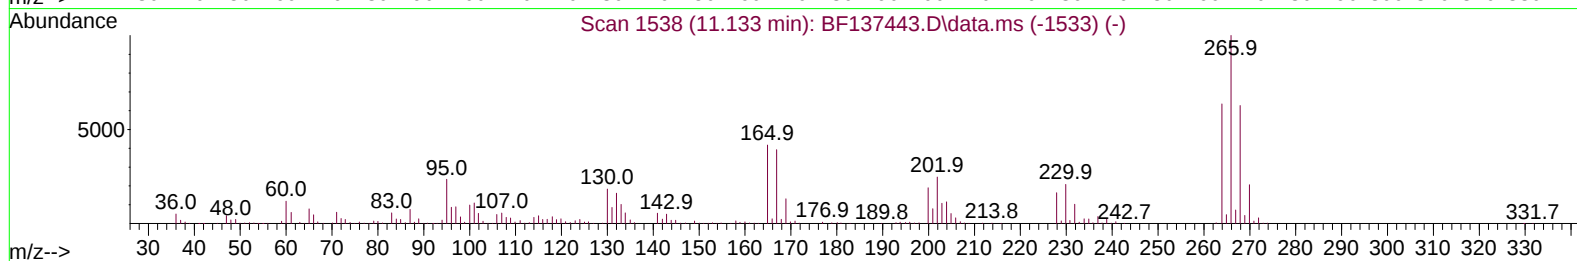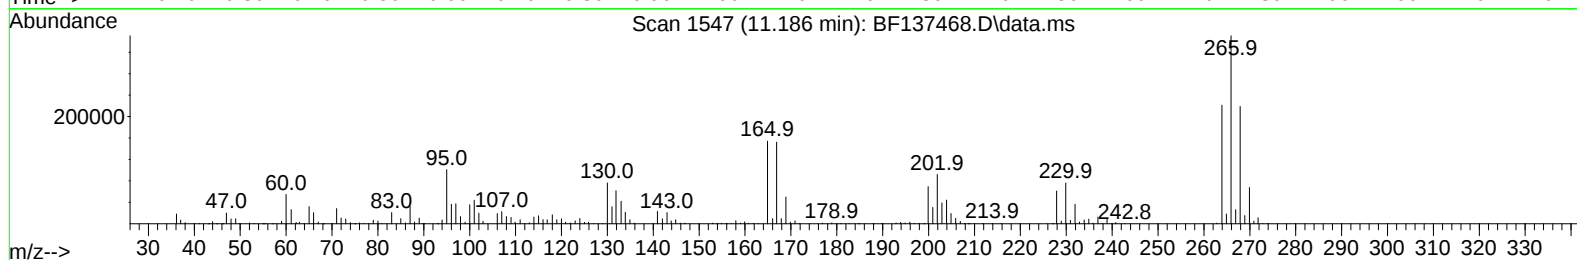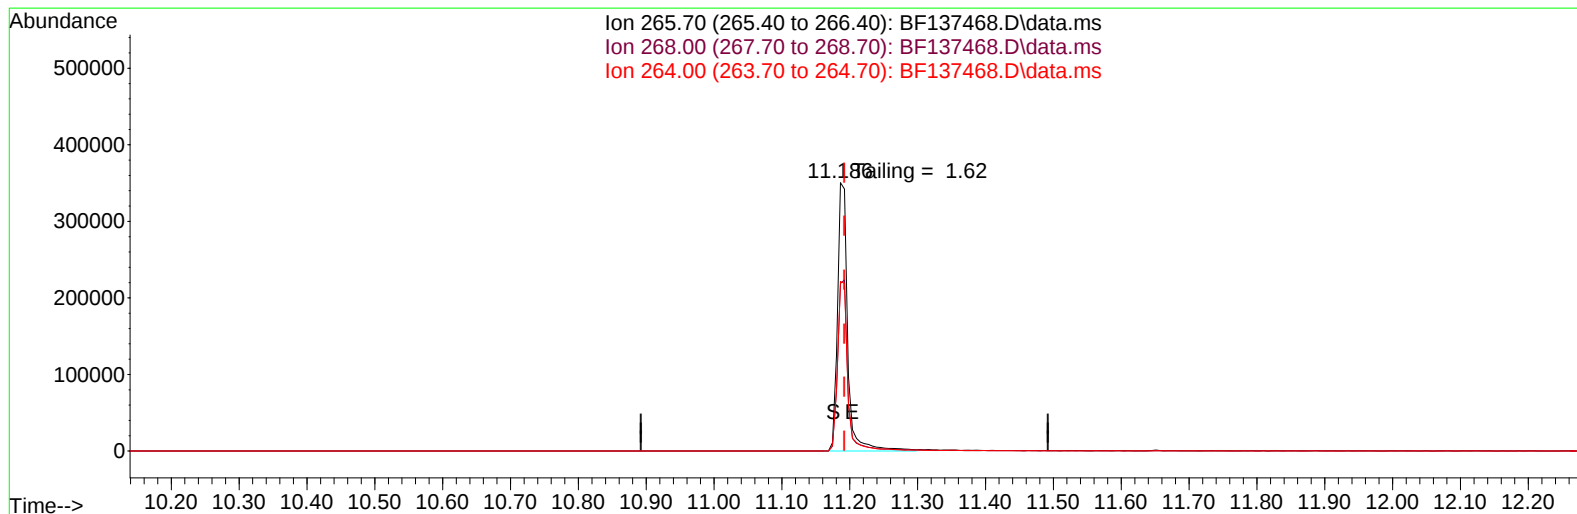

TIC: BF137468.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 297847.57 ng

response 364459

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.41
264.00	63.60	63.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/2/2024	BNA_F	<u>BF137468.D</u>
Compound Name	Response	Retention Time
DDT	774563	13.568
DDD	10716	13.292
DDE	1059	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11775	786338	1.50

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP