


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030315\
 Data File : BF077541.D
 Acq On : 3 Mar 2015 11:10
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 02 17:05:52 2015

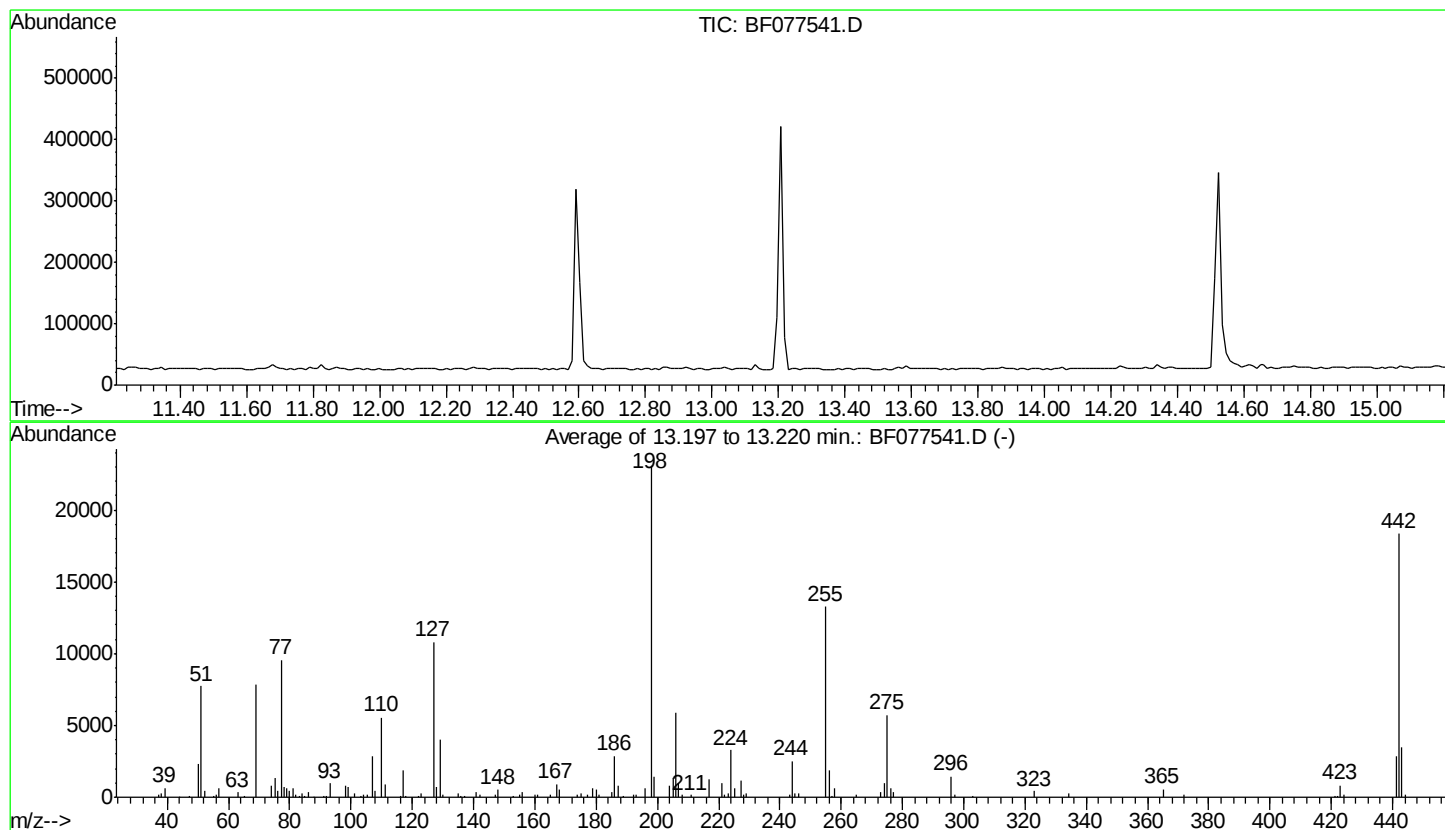

AutoFind: Scans 1077, 1078, 1079; Background Corrected with Scan 1074

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	7740	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.9	7840	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	10819	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23093	PASS
199	198	5	9	6.4	1470	PASS
275	198	10	60	24.7	5706	PASS
365	198	1	100	2.5	569	PASS
441	442	0.01	24	15.7	2883	PASS
442	198	50	100	79.4	18341	PASS
443	442	15	24	18.8	3442	PASS