


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030316\
 Data File : BF085176.D
 Acq On : 4 Mar 2016 00:30
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 04 00:54:58 2016

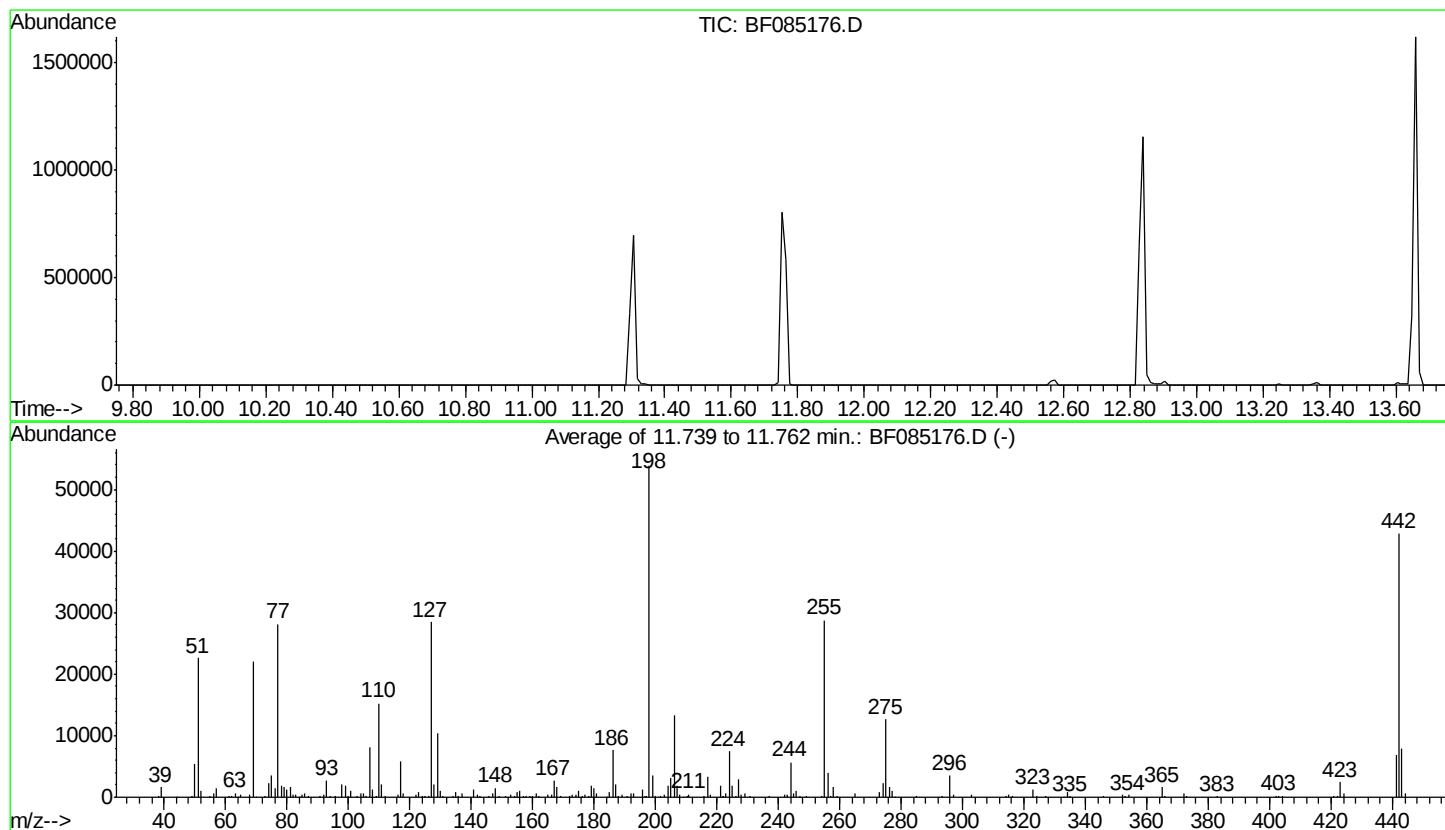

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	22595	PASS
68	69	0.00	2	1.7	366	PASS
69	198	0.00	100	41.0	22109	PASS
70	69	0.00	2	0.5	103	PASS
127	198	10	80	52.8	28421	PASS
197	198	0.00	2	0.3	178	PASS
198	198	100	100	100.0	53860	PASS
199	198	5	9	6.7	3634	PASS
275	198	10	60	23.5	12638	PASS
365	198	1	100	3.0	1596	PASS
441	442	0.01	24	15.9	6796	PASS
442	198	50	100	79.5	42820	PASS
443	442	15	24	18.7	8004	PASS