
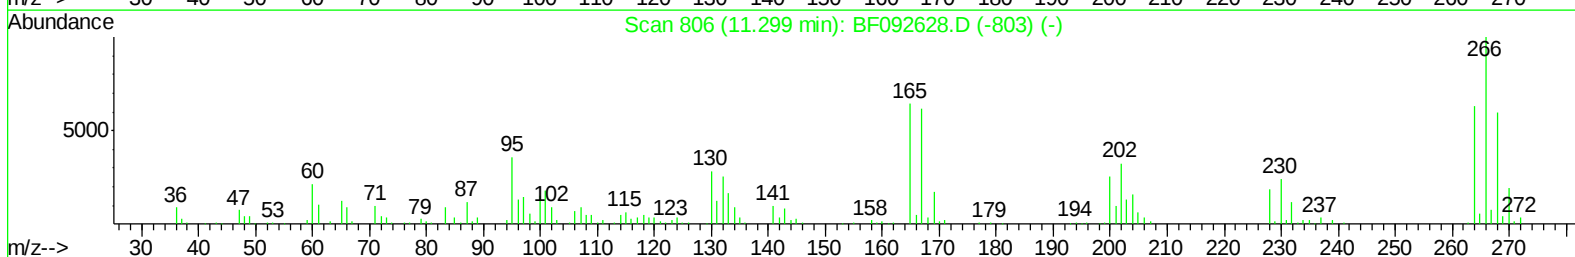
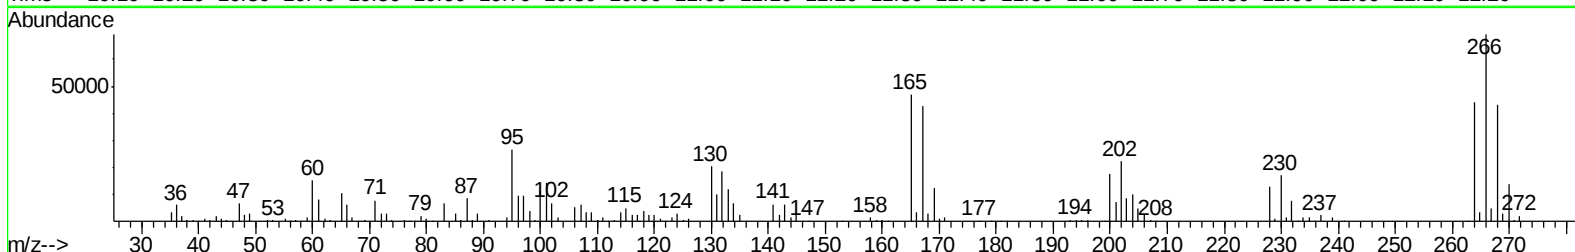


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030317\
Data File : BF093362.D
Acq On : 3 Mar 2017 16:25
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 05:48:45 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

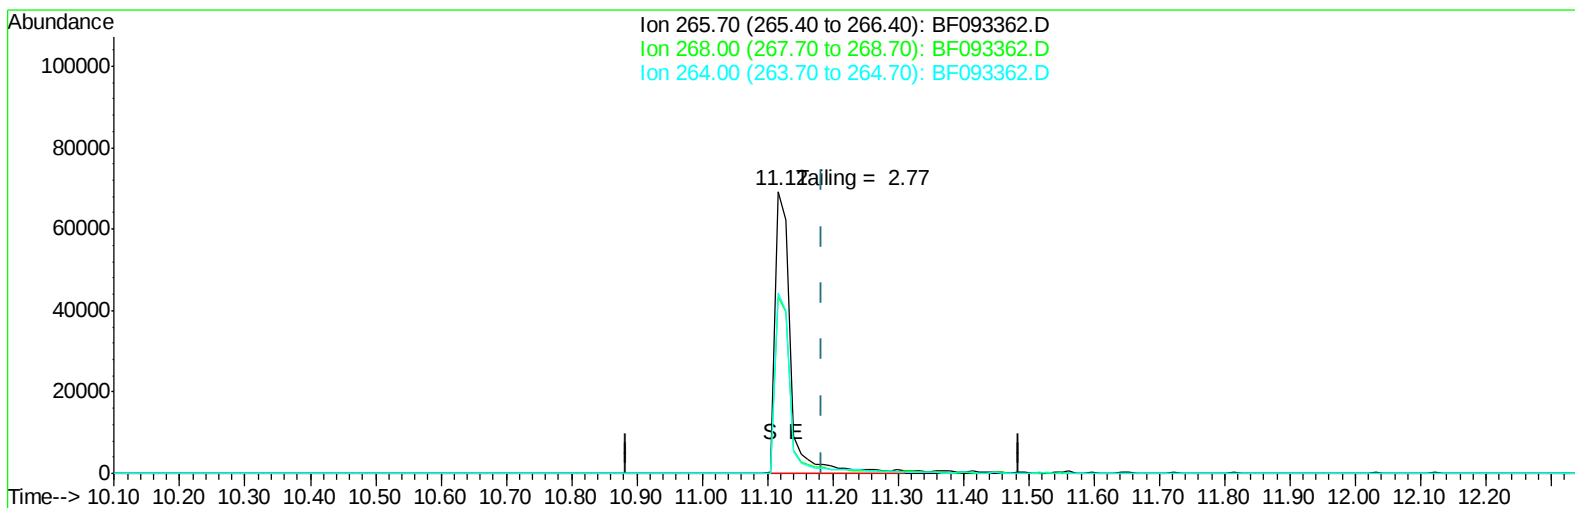

TIC: BF093362.D

(69) Pentachlorophenol (C)

11.116min (-0.069) 51649.70ng

response 114333

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	62.82
264.00	62.90	64.01
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030317\  
Data File : BF093362.D  
Acq On    : 3 Mar 2017 16:25  
Operator  : SJ/MA  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Data File : BF093362.D

Acq On : 3 Mar 2017 16:25

Operator : SJ/MA

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1


Quant Time: Mar 04 05:48:45 2017

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 17 17:31:55 2017

Response via : Initial Calibration

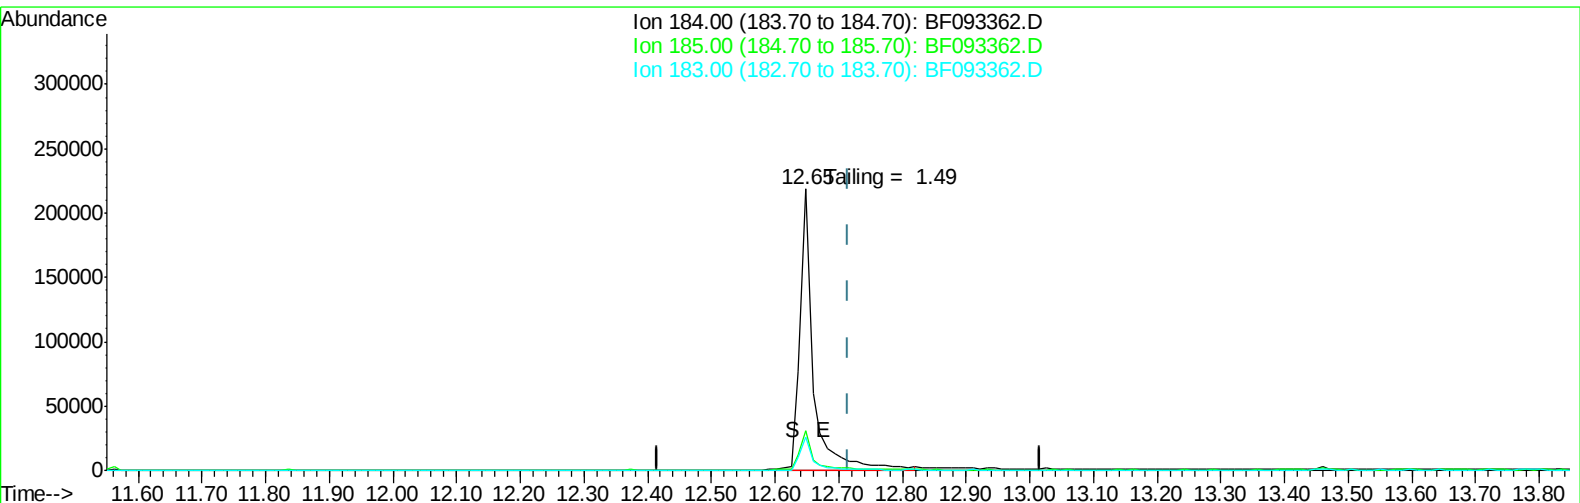

lon 184.00 (183.70 to 184.70): BF093362.D


Ion 185.00 (184.70 to 185.70): BF093362.D

Ion 183.00 (182.70 to 183.70): BF093362.D


12.65 $t_{\text{ailing}} = 1.49$

Failing = 1.49

Time--> 11.60 11.70 11.80 11.90 12.00 12.10 12.20 12.30 12.40 12.50 12.60 12.70 12.80 12.90 13.00 13.10 13.20 13.30 13.40 13.50 13.60 13.70 13.80

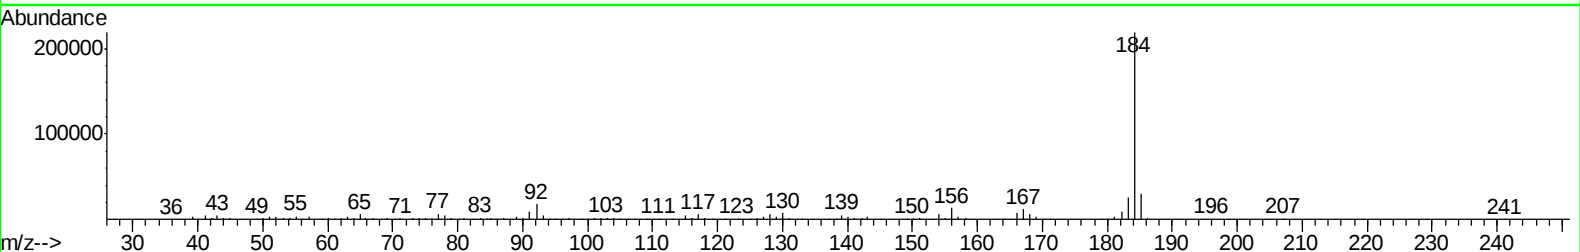

m/z--> 30 40 50 60 70 80 90 100 110 120 130 140 150 160 170 180 190 200 210 220 230 240

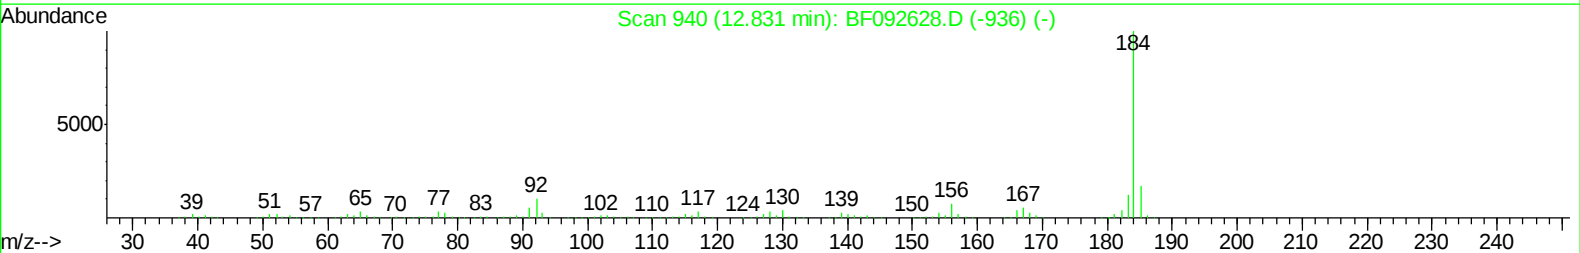

Scan 940 (12.831 min): BF092628.D (-936) (-)

m/z--> 30 40 50 60 70 80 90 100 110 120 130 140 150 160 170 180 190 200 210 220 230 240

TIC: BF093362.D

(76) Benzidine

12.648min (-0.069) 0.00ng

response 328465

Ion	Exp%	Act%
-----	------	------

184.00	100	100
--------	-----	-----

185.00	16.70	14.14
--------	-------	-------

183.00	11.50	11.96
--------	-------	-------

0.00 0.00 0.00