
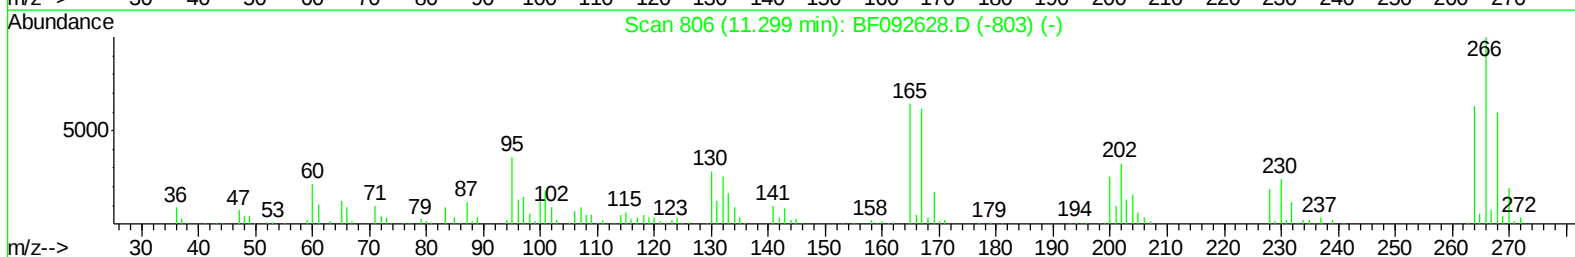
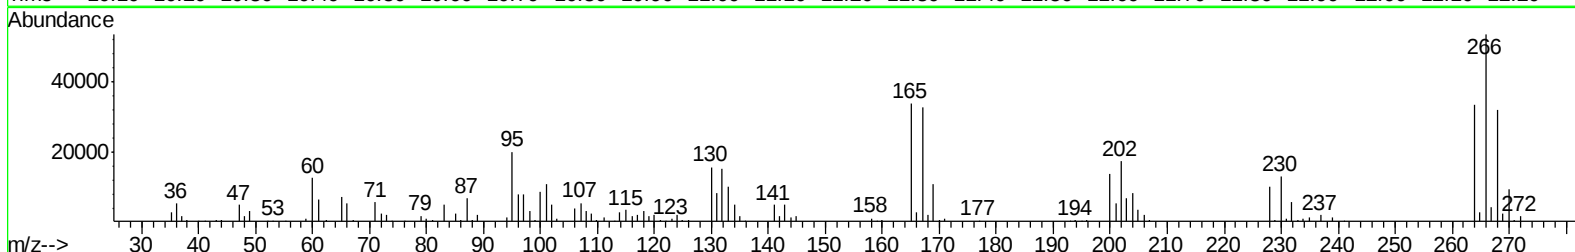


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030317\
Data File : BF093385.D
Acq On : 4 Mar 2017 4:47
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 05:49:32 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

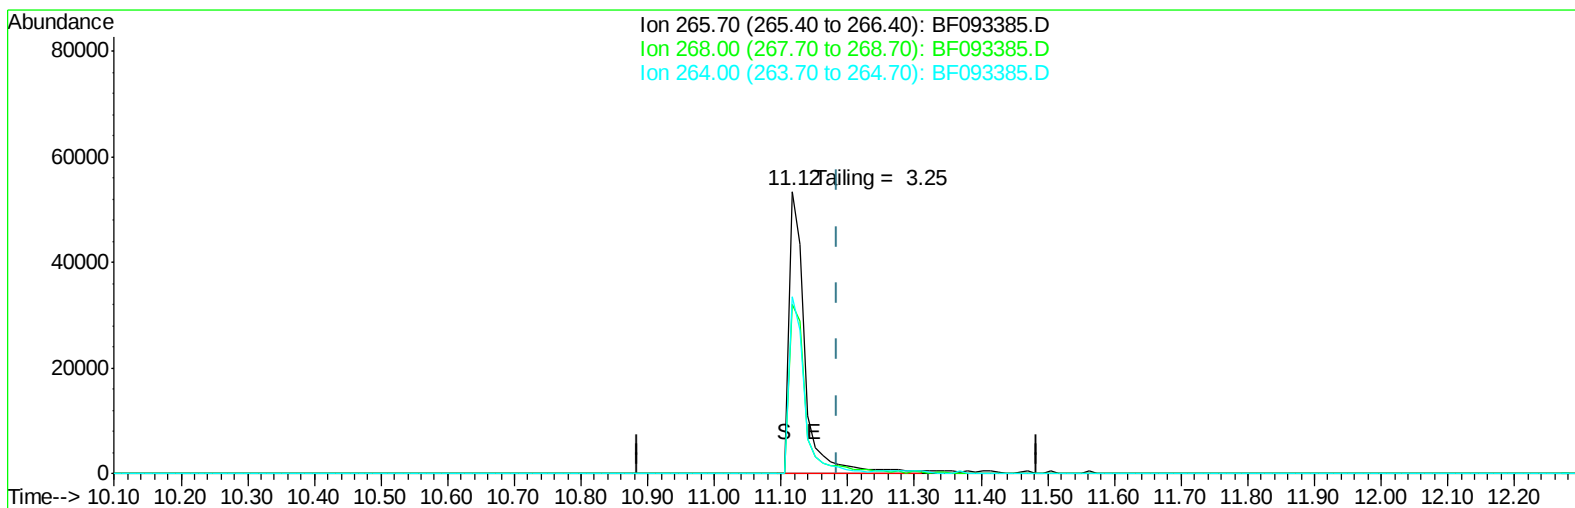

TIC: BF093385.D

(69) Pentachlorophenol (C)

11.116min (-0.069) 30985.76ng

response 88180

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	59.79
264.00	62.90	62.70
0.00	0.00	0.00

