

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030317\
 Data File : BF093371.D
 Acq On : 3 Mar 2017 21:01
 Operator : SJ/MA
 Sample : I2086-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SRI-MW-4-20170302

Quant Time: Mar 03 23:06:24 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 03 22:55:05 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.78	152	185730	20.00	ng	0.00
21) Naphthalene-d8	8.08	136	708294	20.00	ng	0.00
38) Acenaphthene-d10	9.82	164	357737	20.00	ng	0.00
63) Phenanthrene-d10	11.30	188	629646	20.00	ng	-0.01
75) Chrysene-d12	13.94	240	533395	20.00	ng	-0.01
86) Perylene-d12	15.36	264	394305	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	758568	70.07	ng	0.00
7) Phenol-d6	6.43	99	641145	46.03	ng	-0.01
23) Nitrobenzene-d5	7.36	82	1094445	86.05	ng	-0.01
41) 2,4,6-Tribromophenol	10.61	330	334001	129.09	ng	0.00
44) 2-Fluorobiphenyl	9.15	172	1942662	98.38	ng	0.00
78) Terphenyl-d14	12.89	244	1427570	62.89	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.54	163	84131	3.49	ng	Qvalue # 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF030317\
Data File : BF093371.D
Acq On : 3 Mar 2017 21:01
Operator : SJ/MA
Sample : I2086-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SRI-MW-4-20170302

Quant Time: Mar 03 23:06:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 03 22:55:05 2017
Response via : Initial Calibration

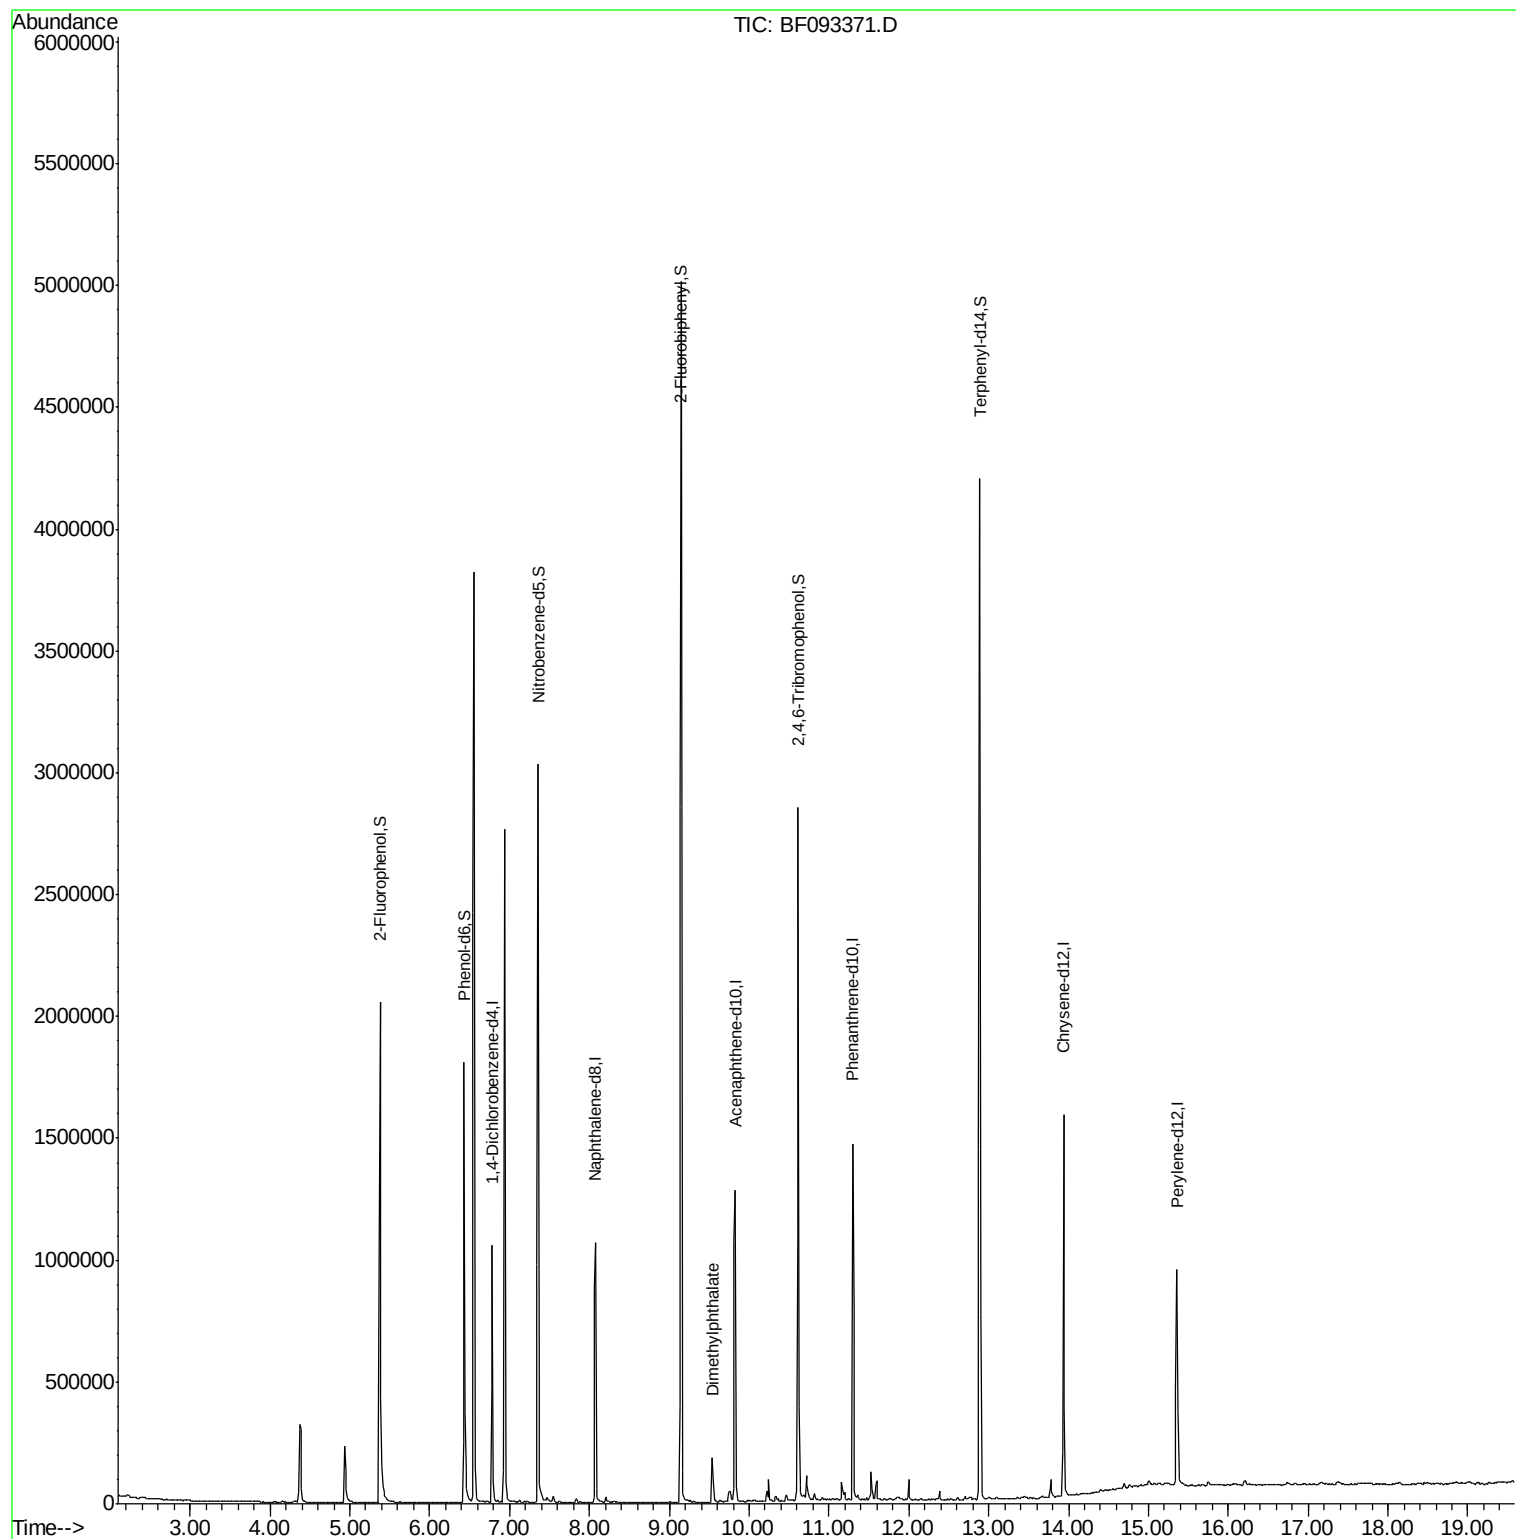




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.78 min Scan# 411
Delta R.T. -0.00 min
Lab File: BF093371.D
Acq: 3 Mar 2017 21:01

Instrument :
BNA_F
ClientSampleId :
SRI-MW-4-20170302

Tot Ion:152 Resp: 185730
Ion Ratio Lower Upper
152 100
150 154.7 124.9 187.3
115 55.7 46.0 69.0

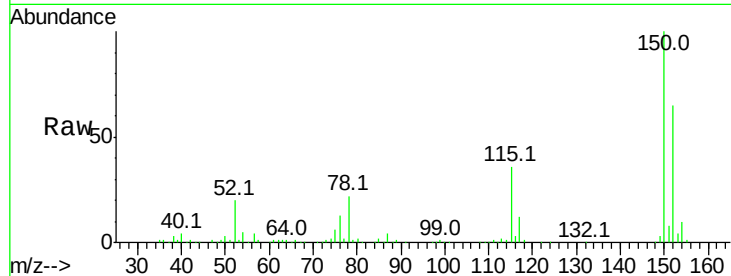


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

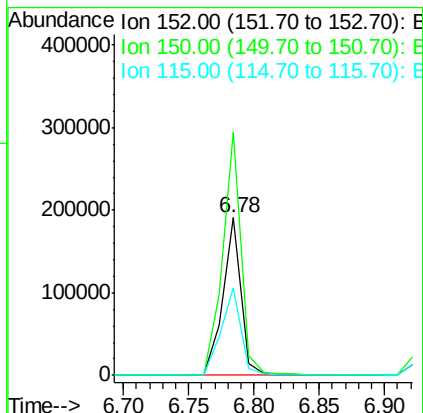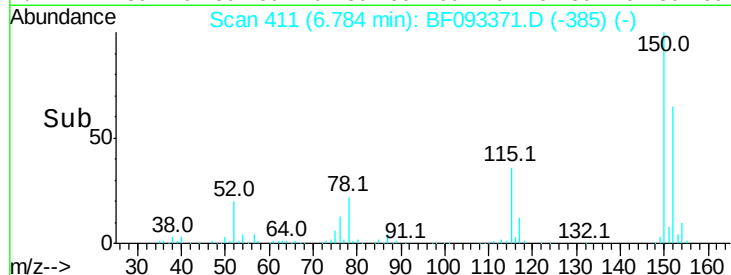



#5


2-Fluorophenol
Concen: 70.07 ng
RT: 5.38 min Scan# 288
Delta R.T. -0.00 min
Lab File: BF093371.D
Acq: 3 Mar 2017 21:01

Tgt Ion:112 Resp: 758568
Ion Ratio Lower Upper
112 100
64 58.4 46.1 69.1
63 28.7 23.8 35.6



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

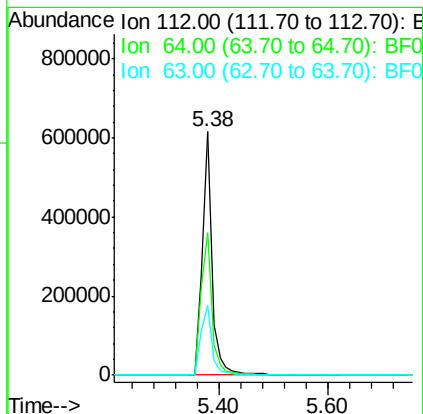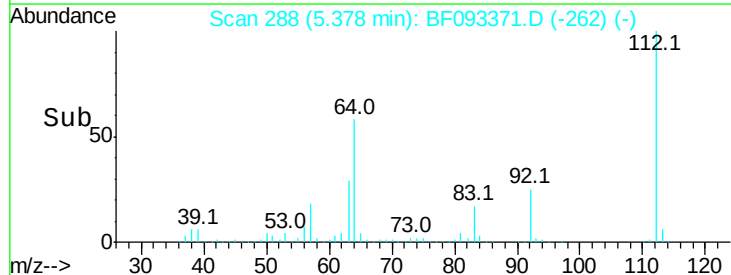

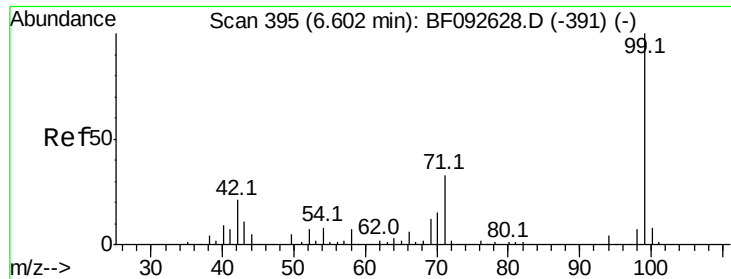

#7

Phenol-d6

Concen: 46.03 ng

RT: 6.43 min Scan# 380

Delta R.T. -0.01 min

Lab File: BF093371.D

Acq: 3 Mar 2017 21:01

Instrument :

BNA_F

ClientSampleId :

SRI-MW-4-20170302


Tot Ion: 99 Resp: 641145

Ion Ratio Lower Upper

99 100

42 19.4 15.6 23.4




71 31.0 27.5 41.3

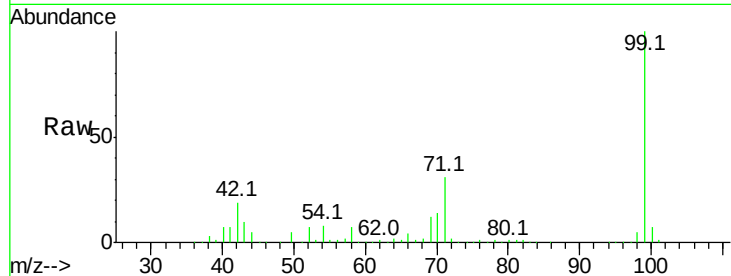

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

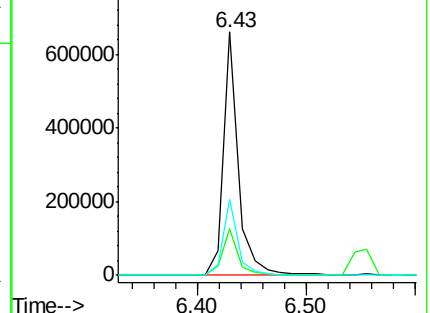

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.08 min Scan# 524

Delta R.T. -0.00 min

Lab File: BF093371.D

Acq: 3 Mar 2017 21:01

Tgt Ion: 136 Resp: 708294


Ion Ratio Lower Upper

136 100

137 10.5 8.4 12.6

54 7.1 4.5 6.7#

68 5.2 3.6 5.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

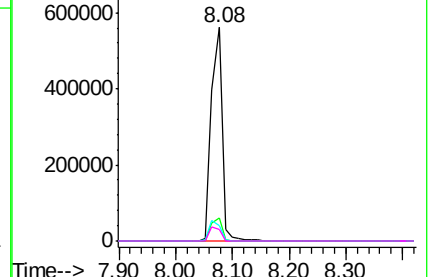







#23
 Nitrobenzene-d5
 Concen: 86.05 ng
 RT: 7.36 min Scan# 461
 Delta R.T. -0.01 min
 Lab File: BF093371.D
 Acq: 3 Mar 2017 21:01

Instrument :
 BNA_F
 ClientSampleId :
 SRI-MW-4-20170302

Tot Ion: 82 Resp: 1094445
 Ion Ratio Lower Upper
 82 100
 128 41.3 34.6 52.0
 54 58.8 39.5 59.3

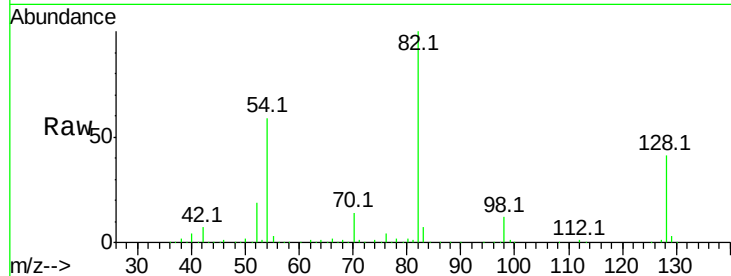


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0


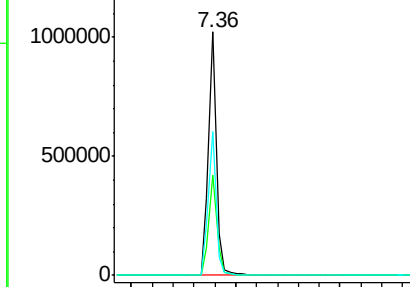



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.82 min Scan# 677
 Delta R.T. -0.00 min
 Lab File: BF093371.D
 Acq: 3 Mar 2017 21:01

Tgt Ion:164 Resp: 357737
 Ion Ratio Lower Upper
 164 100
 162 105.2 80.2 120.2
 160 47.1 36.9 55.3



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

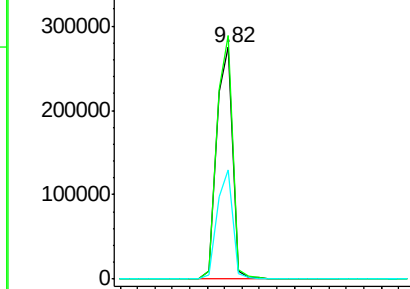







#41
 2,4,6-Tribromophenol
 Concen: 129.09 ng
 RT: 10.61 min Scan# 746
 Delta R.T. -0.00 min
 Lab File: BF093371.D
 Acq: 3 Mar 2017 21:01

Instrument :
 BNA_F
 ClientSampleId :
 SRI-MW-4-20170302

Tot Ion:330 Resp: 334001
 Ion Ratio Lower Upper
 330 100
 332 97.3 77.4 116.2
 141 41.9 34.1 51.1

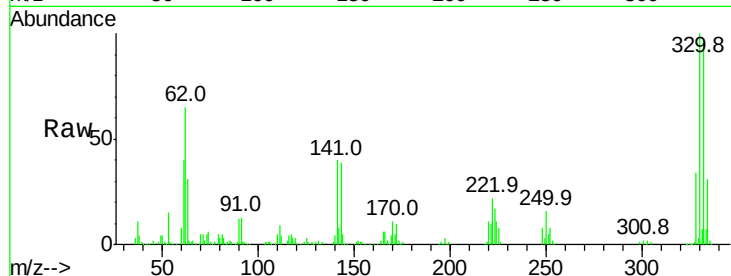


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


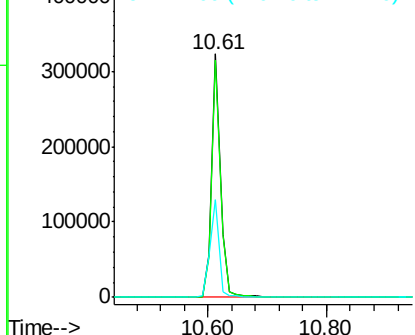



#44
 2-Fluorobiphenyl
 Concen: 98.38 ng
 RT: 9.15 min Scan# 618
 Delta R.T. -0.00 min
 Lab File: BF093371.D
 Acq: 3 Mar 2017 21:01

Tgt Ion:172 Resp: 1942662
 Ion Ratio Lower Upper
 172 100
 171 37.5 29.4 44.0
 170 24.9 20.2 30.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

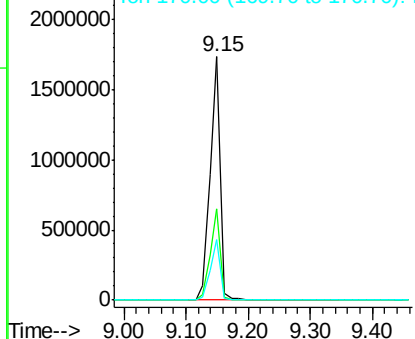

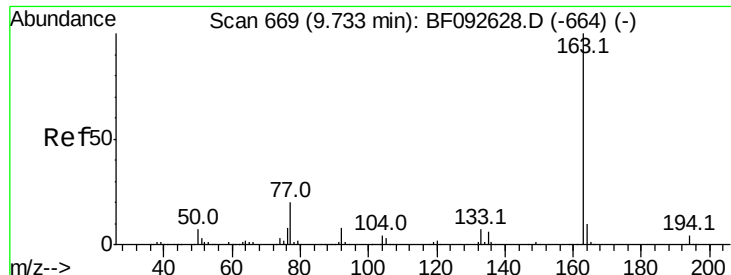

#49

Dimethylphthalate

Concen: 3.49 ng

RT: 9.54 min Scan# 652

Delta R.T. -0.01 min

Lab File: BF093371.D

Acq: 3 Mar 2017 21:01

Instrument :

BNA_F

ClientSampleId :

SRI-MW-4-20170302


Tot Ion:163 Resp: 84131

Ion Ratio Lower Upper

163 100

194 2.8 3.0 4.4#




164 10.4 8.0 12.0



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

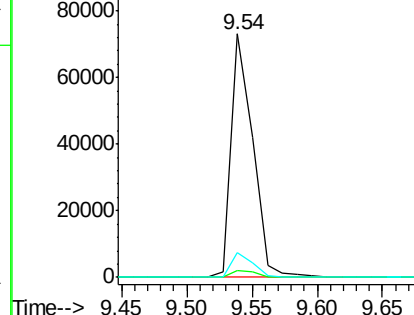

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.30 min Scan# 806

Delta R.T. -0.01 min

Lab File: BF093371.D

Acq: 3 Mar 2017 21:01


Tgt Ion:188 Resp: 629646

Ion Ratio Lower Upper

188 100

94 14.3 10.0 15.0



80 15.5 11.2 16.8




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

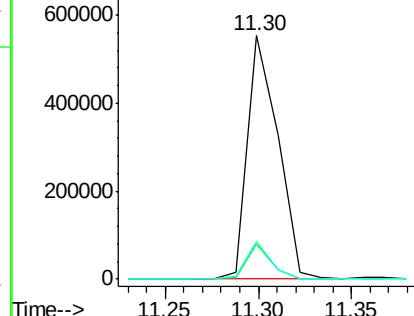



#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.94 min Scan# 1037

Delta R.T. -0.01 min

Lab File: BF093371.D

Acq: 3 Mar 2017 21:01

Instrument :

BNA_F

ClientSampleId :

SRI-MW-4-20170302


Tot Ion:240 Resp: 533395

Ion Ratio Lower Upper

240 100

120 15.6 12.9 19.3




236 26.1 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

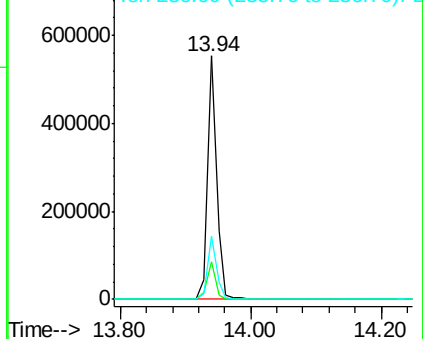

#78

Terphenyl-d14

Concen: 62.89 ng

RT: 12.89 min Scan# 945

Delta R.T. -0.00 min

Lab File: BF093371.D

Acq: 3 Mar 2017 21:01


Tgt Ion:244 Resp: 1427570

Ion Ratio Lower Upper

244 100

212 7.7 6.2 9.2



122 13.8 11.4 17.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

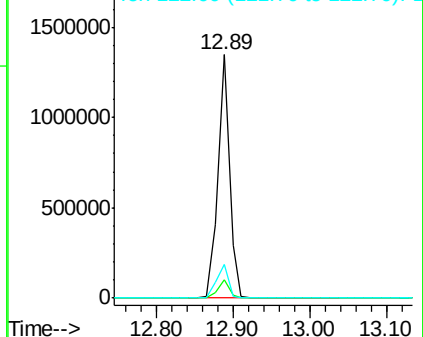


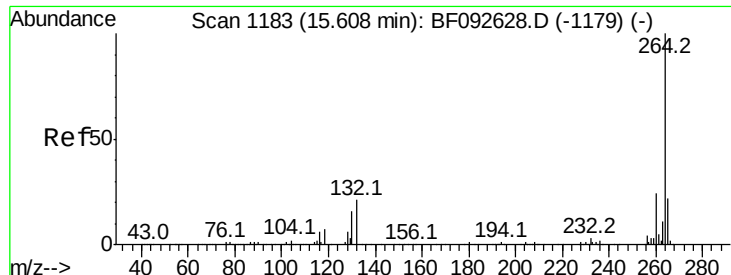

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.36 min Scan# 1161
 Delta R.T. -0.01 min
 Lab File: BF093371.D
 Acq: 3 Mar 2017 21:01

Instrument :
 BNA_F
 ClientSampleId :
 SRI-MW-4-20170302

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.2	28.8
265	21.5	17.4	26.0

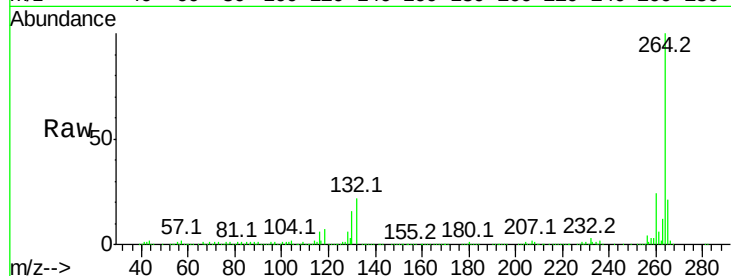

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

