


Data Path : Z:\HPCHEM1\BNA F\Data\BF030317\
 Data File : BF093362.D
 Acq On : 3 Mar 2017 16:25
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 17:31:55 2017

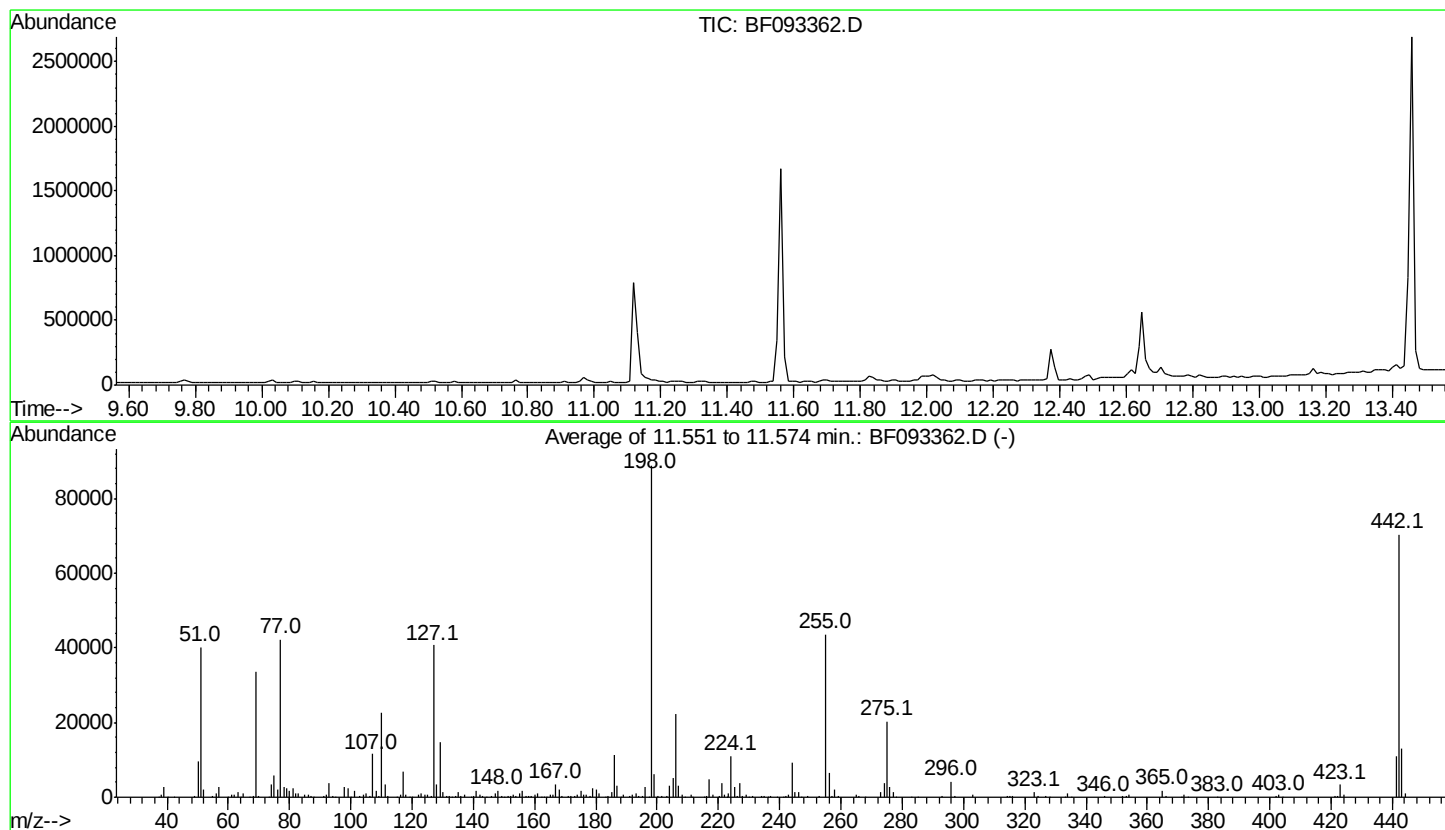

AutoFind: Scans 828, 829, 830; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	40257	PASS
68	69	0.00	2	1.3	428	PASS
69	198	0.00	100	37.9	33631	PASS
70	69	0.00	2	1.0	323	PASS
127	198	10	80	45.8	40672	PASS
197	198	0.00	2	0.1	131	PASS
198	198	100	100	100.0	88757	PASS
199	198	5	9	7.0	6169	PASS
275	198	10	60	22.9	20366	PASS
365	198	1	100	1.9	1718	PASS
441	442	0.01	24	15.4	10842	PASS
442	198	50	100	79.2	70321	PASS
443	442	15	24	18.7	13124	PASS