

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
 Data File : BF127174.D
 Acq On : 03 Mar 2022 16:39
 Operator : CG\JU
 Sample : N1689-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-40

Quant Time: Mar 04 02:13:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 01 23:57:09 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.886	152	79252	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	323067	20.000	ng	# 0.00
39) Acenaphthene-d10	9.933	164	168014	20.000	ng	0.00
64) Phenanthrene-d10	11.421	188	285111	20.000	ng	# 0.00
76) Chrysene-d12	14.068	240	152011	20.000	ng	# 0.00
86) Perylene-d12	15.556	264	147838	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	313930	61.223	ng	0.00
7) Phenol-d6	6.516	99	249499	36.060	ng	0.00
23) Nitrobenzene-d5	7.457	82	638061	89.147	ng	0.00
42) 2,4,6-Tribromophenol	10.727	330	286163	147.930	ng	0.00
45) 2-Fluorobiphenyl	9.251	172	1055396	92.475	ng	0.00
79) Terphenyl-d14	13.010	244	1068141	103.296	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propyla...	7.457	70	97787	21.933	ng	# 79
25) Isophorone	7.457	82	634524	53.575	ng	# 69
67) 4-Bromophenyl-phenylether	10.727	248	16709	5.245	ng	# 1
77) Benzidine	13.010	184	16327	3.952	ng	# 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127174.D
Acq On : 03 Mar 2022 16:39
Operator : CG\JU
Sample : N1689-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-40

Quant Time: Mar 04 02:13:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 01 23:57:09 2022
Response via : Initial Calibration




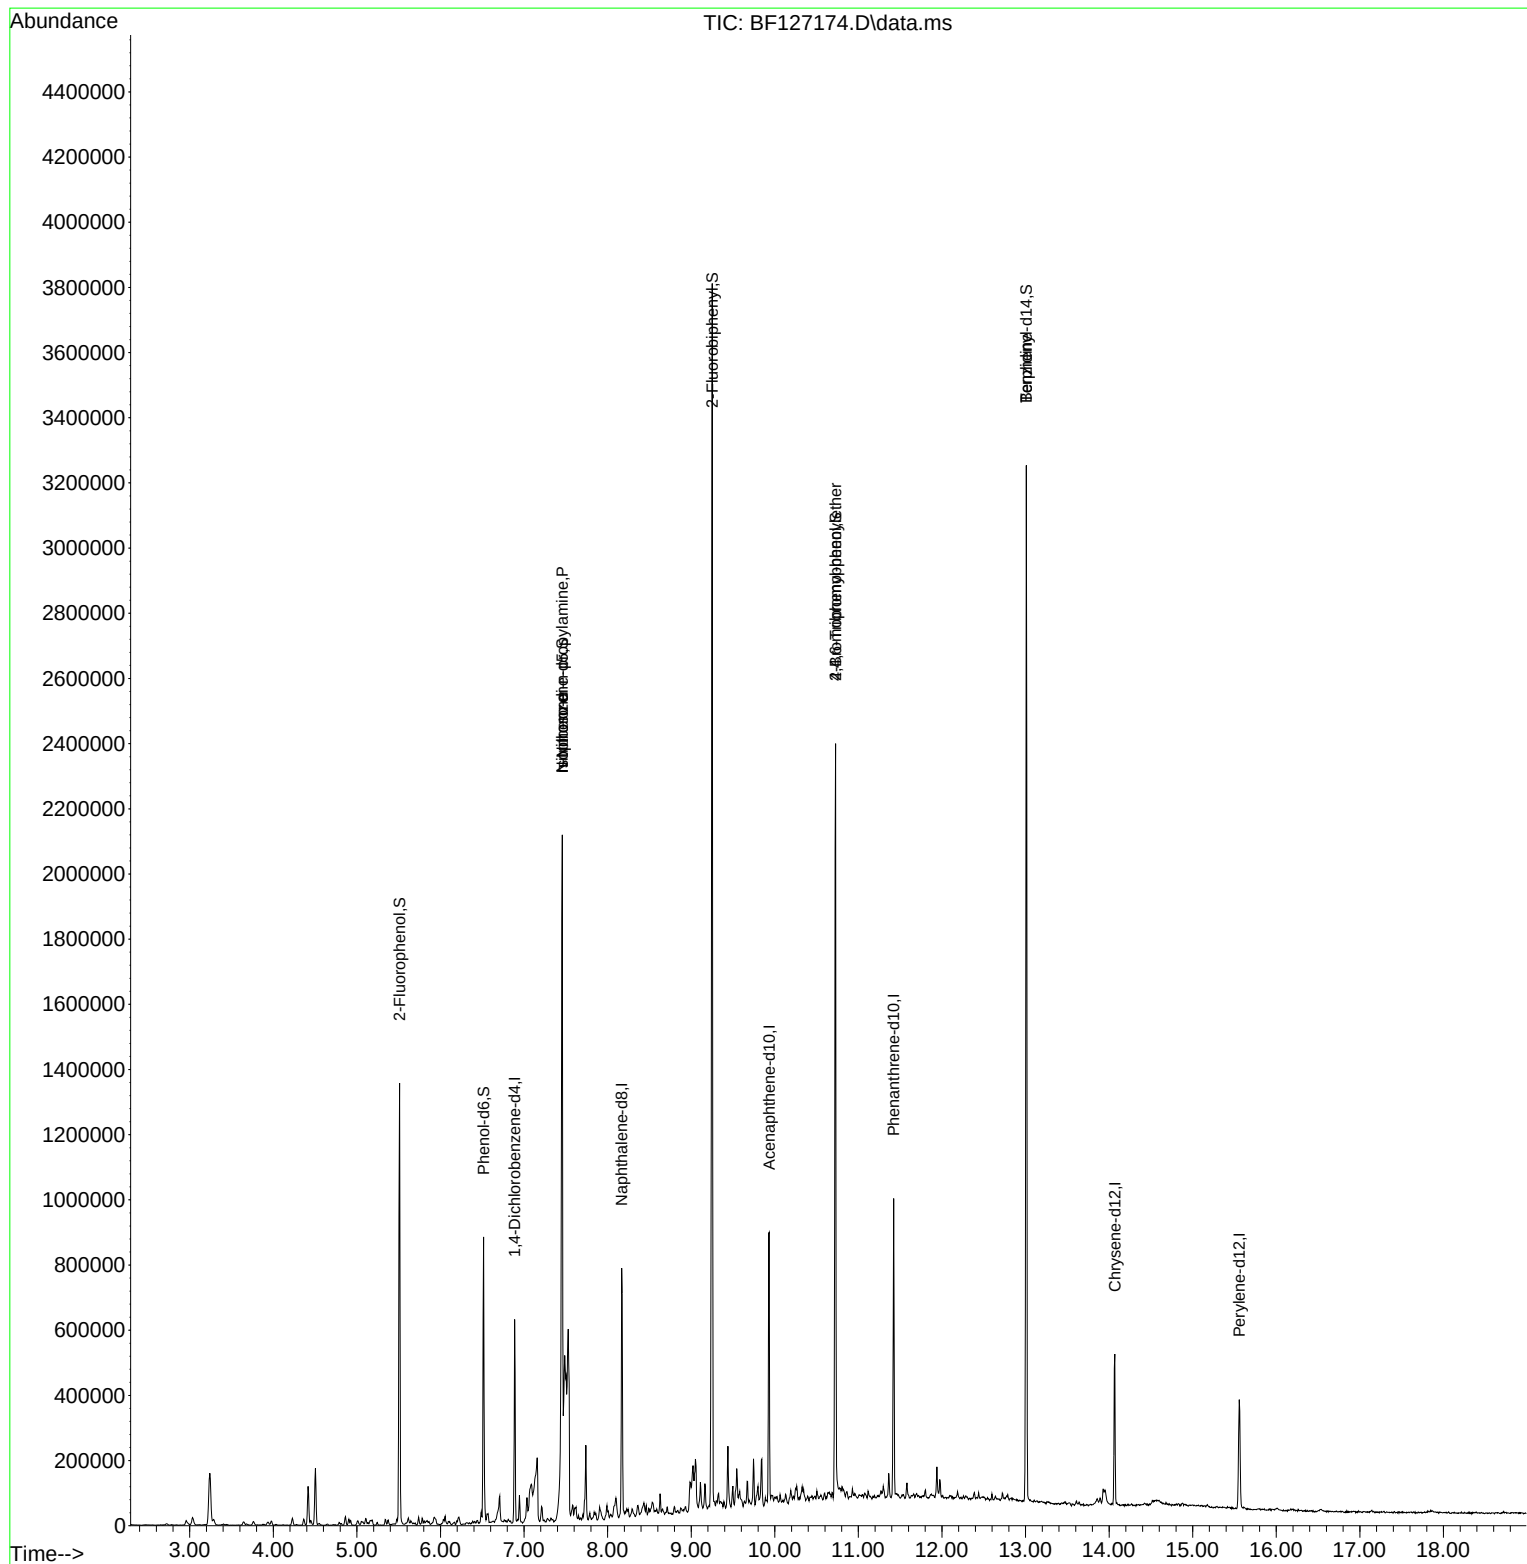


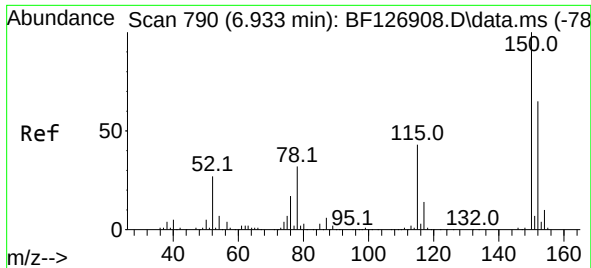

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.886 min Scan# 71
Delta R.T. -0.007 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39




Instrument :
BNA_F
ClientSampleId :
MW-40


Tgt Ion:152 Resp: 79252
Ion Ratio Lower Upper
152 100
150 159.8 128.1 192.1
115 69.7 56.7 85.1

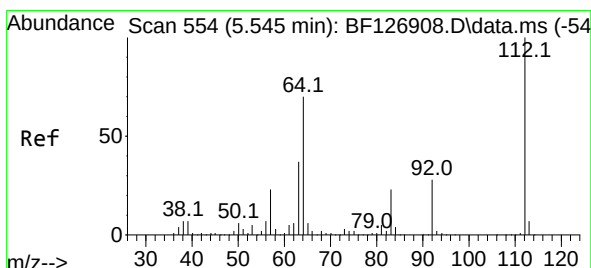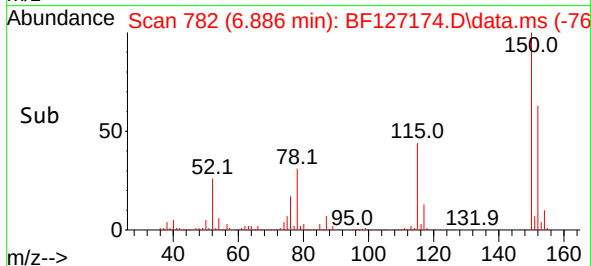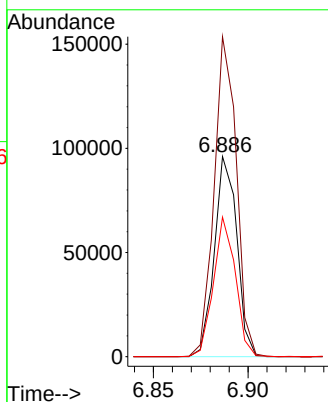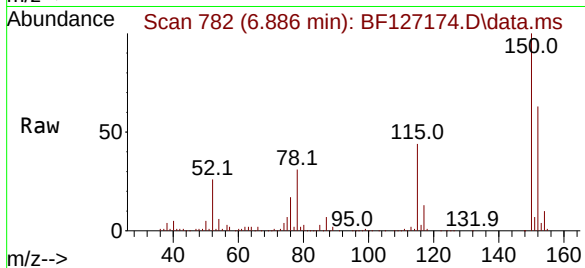

#5
2-Fluorophenol
Concen: 61.223 ng
RT: 5.510 min Scan# 548
Delta R.T. -0.000 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39

Tgt Ion:112 Resp: 313930
Ion Ratio Lower Upper
112 100
64 66.0 49.5 74.3
63 35.3 23.9 35.9


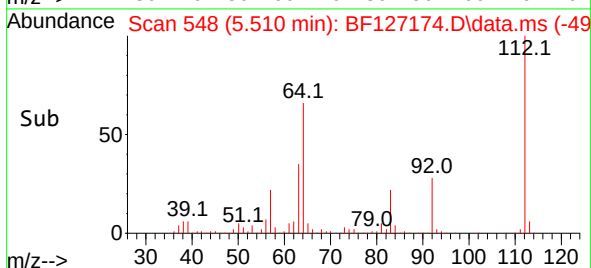
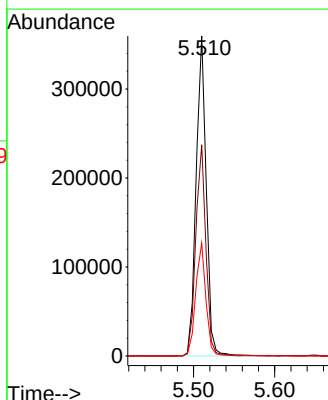
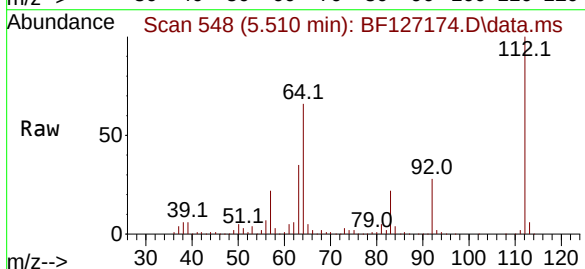


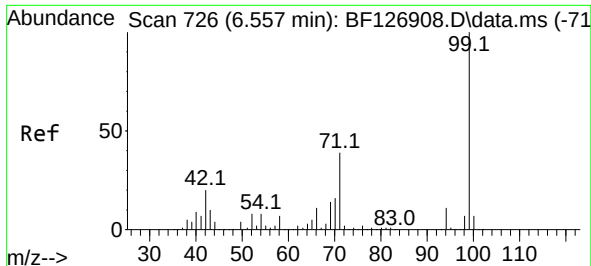

#7
Phenol-d6
Concen: 36.060 ng
RT: 6.516 min Scan# 719
Delta R.T. -0.006 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39




Instrument :
BNA_F
ClientSampleId :
MW-40


Tgt Ion: 99 Resp: 249499
Ion Ratio Lower Upper
99 100
42 19.2 14.2 21.4
71 44.7 24.3 36.5#

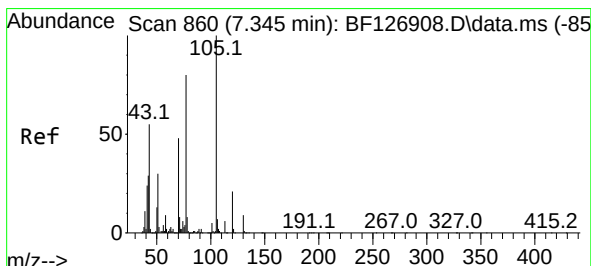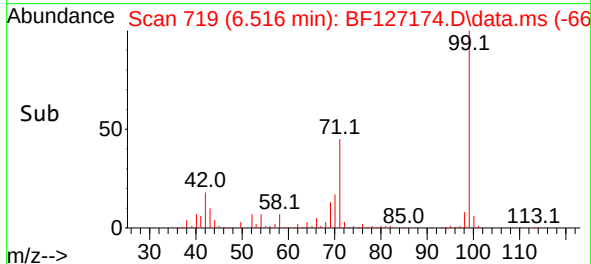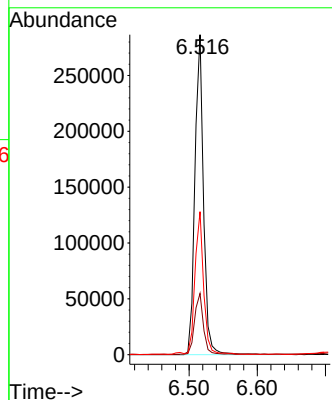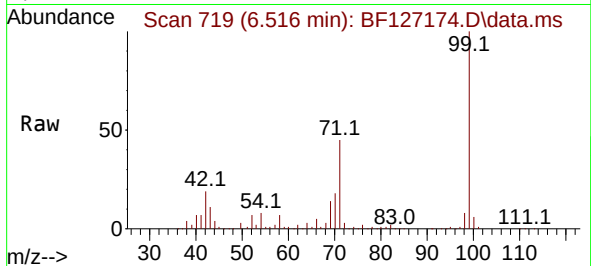

#19
n-Nitroso-di-n-propylamine
Concen: 21.933 ng
RT: 7.457 min Scan# 879
Delta R.T. 0.153 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39

Tgt Ion: 70 Resp: 97787
Ion Ratio Lower Upper
70 100
42 44.7 45.8 68.8#
101 1.8 6.9 10.3#
130 2.1 14.4 21.6#


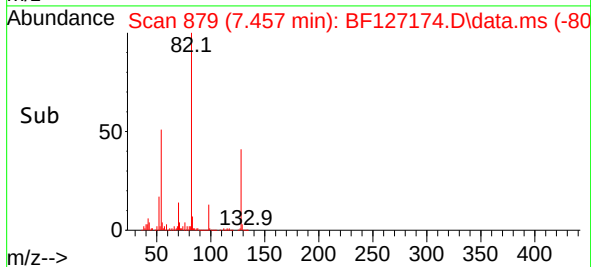
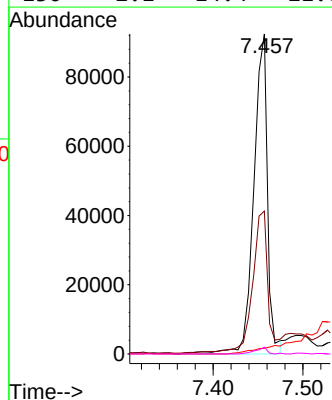
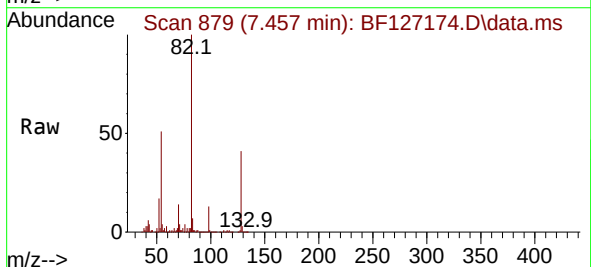


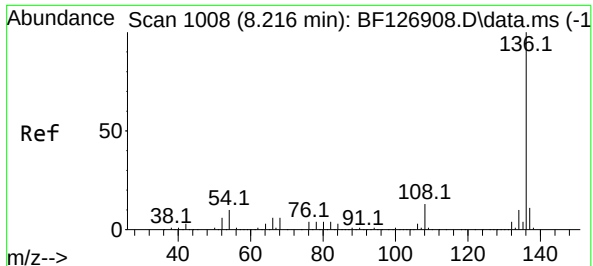

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 10
Delta R.T. -0.006 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39




Instrument :
BNA_F
ClientSampleId :
MW-40


Tgt	Ion:136	Resp:	323067
Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.6	13.0
54	9.5	7.8	11.6
68	5.7	6.3	9.5#

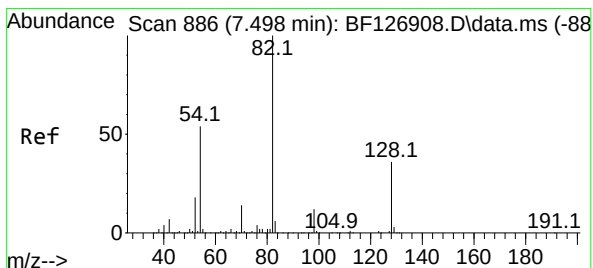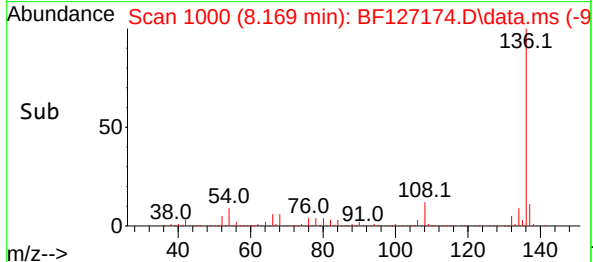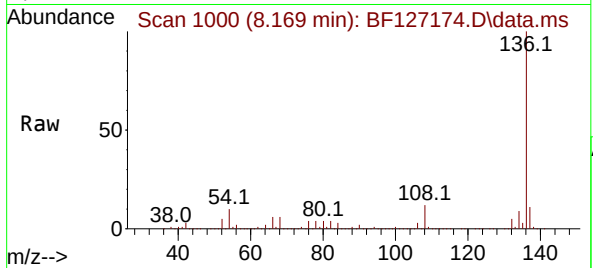

#23
Nitrobenzene-d5
Concen: 89.147 ng
RT: 7.457 min Scan# 879
Delta R.T. -0.006 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39

Tgt Ion: 82	Resp: 638061
Ion Ratio	Lower Upper
82 100	
128 41.4	32.7 49.1
54 51.0	41.7 62.5


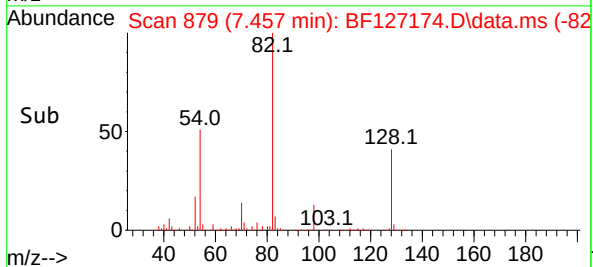

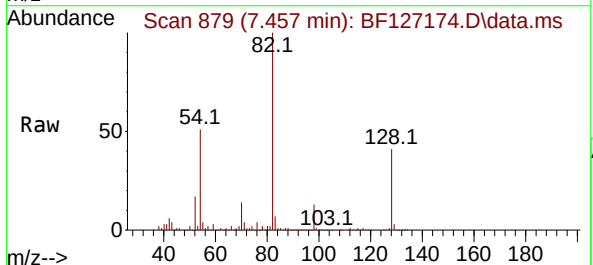


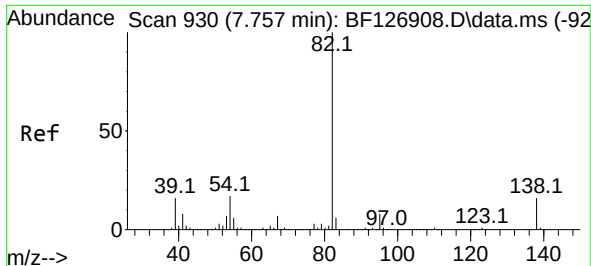

#25
Isophorone
Concen: 53.575 ng
RT: 7.457 min Scan# 81
Delta R.T. -0.259 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39




Instrument :
BNA_F
ClientSampleId :
MW-40


Tgt Ion: 82 Resp: 634524
Ion Ratio Lower Upper
82 100
95 0.0 5.0 7.4#
138 0.0 12.3 18.5#

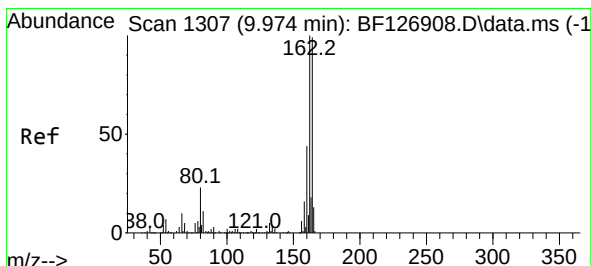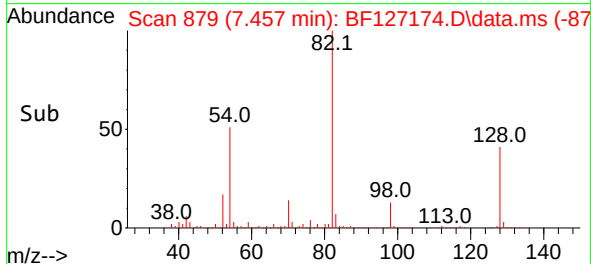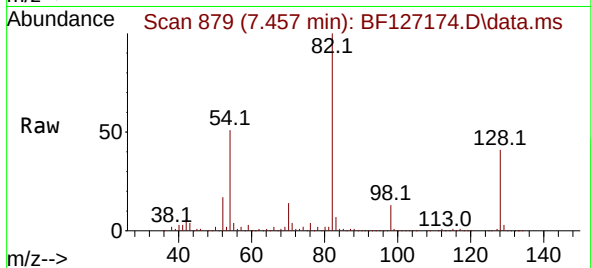

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.933 min Scan# 1300
Delta R.T. -0.006 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39

Tgt Ion:164 Resp: 168014
Ion Ratio Lower Upper
164 100
162 101.1 81.4 122.0
160 46.9 36.6 54.8

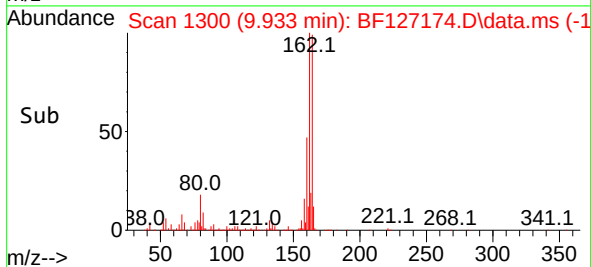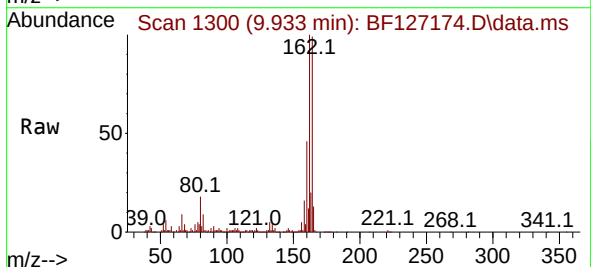

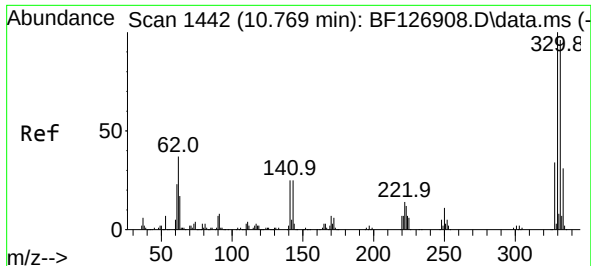

#42

2,4,6-Tribromophenol

Concen: 147.930 ng

RT: 10.727 min Scan# 1442

Delta R.T. -0.000 min

Lab File: BF127174.D

Acq: 03 Mar 2022 16:39

Instrument :

BNA_F

ClientSampleId :

MW-40





Tgt Ion:330 Resp: 286163

Ion Ratio Lower Upper

330 100

332 97.0 76.0 114.0

141 34.9 30.1 45.1

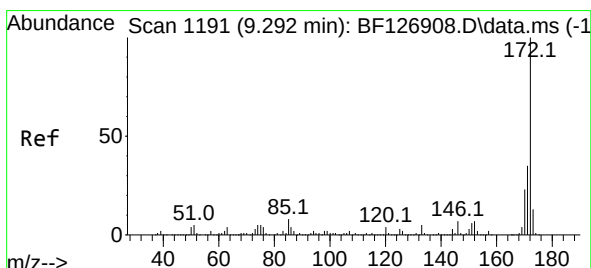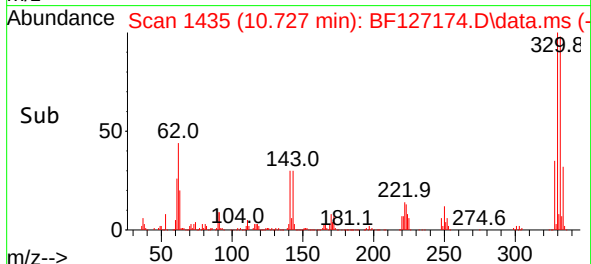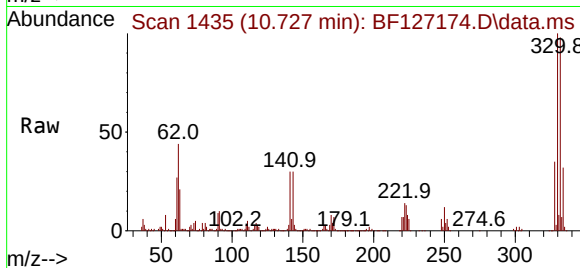

#45

2-Fluorobiphenyl

Concen: 92.475 ng

RT: 9.251 min Scan# 1184

Delta R.T. -0.000 min

Lab File: BF127174.D

Acq: 03 Mar 2022 16:39




Tgt Ion:172 Resp: 1055396


Ion Ratio Lower Upper

172 100

171 35.2 28.3 42.5

170 22.9 19.0 28.6


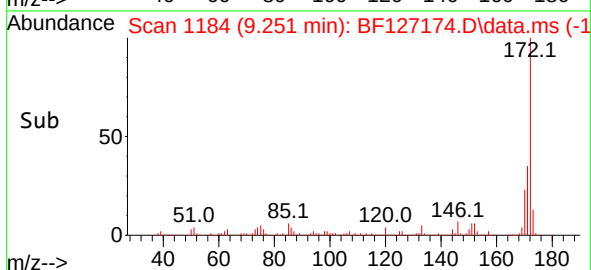

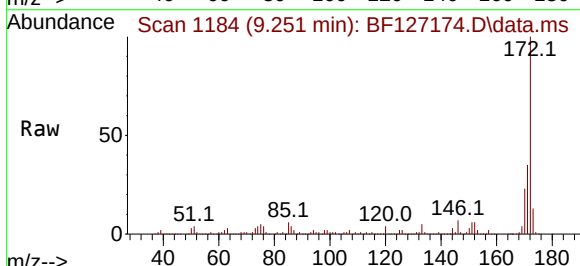


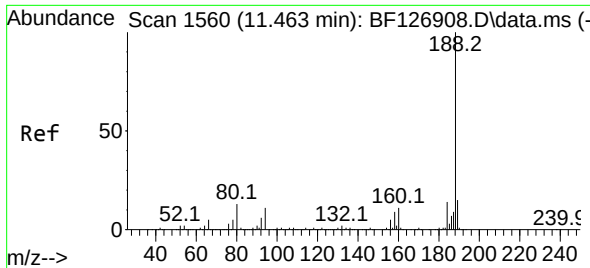

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.421 min Scan# 1
Delta R.T. -0.006 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39




Instrument :
BNA_F
ClientSampleId :
MW-40


Tgt Ion:188 Resp: 285111
Ion Ratio Lower Upper
188 100
94 9.4 10.1 15.1#
80 10.9 11.8 17.6#

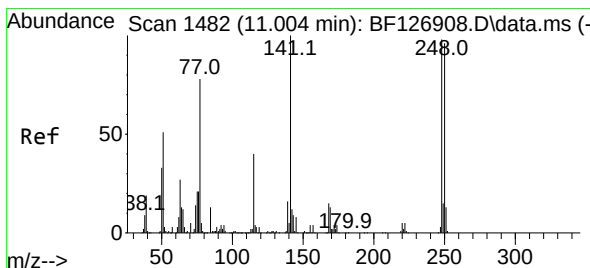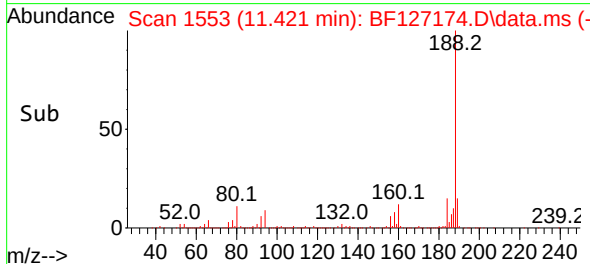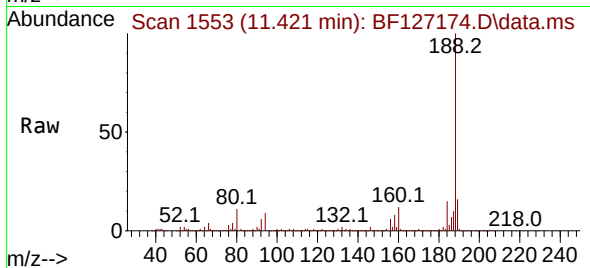

#67
4-Bromophenyl-phenylether
Concen: 5.245 ng
RT: 10.727 min Scan# 1435
Delta R.T. -0.241 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39

Tgt Ion:248 Resp: 16709
Ion Ratio Lower Upper
248 100
250 210.1 76.2 114.4#
141 535.9 66.2 99.4#


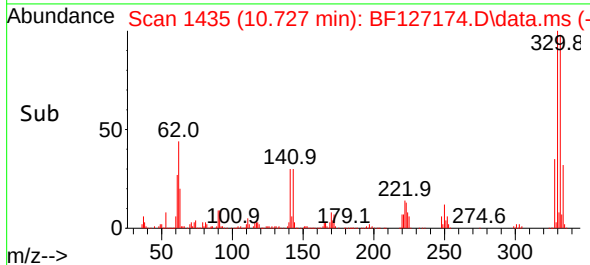

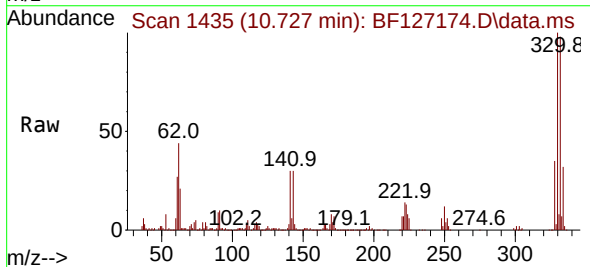


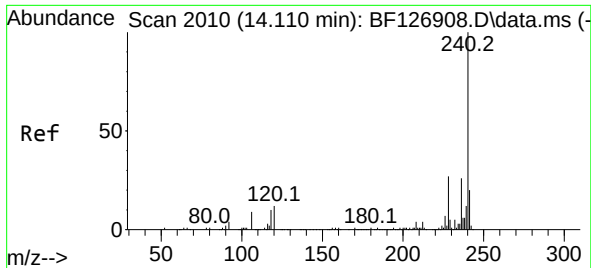

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.068 min Scan# 2010
Delta R.T. -0.006 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39




Instrument :
BNA_F
ClientSampleId :
MW-40


Tgt Ion:240 Resp: 152011
Ion Ratio Lower Upper
240 100
120 9.0 14.4 21.6#
236 26.1 20.5 30.7

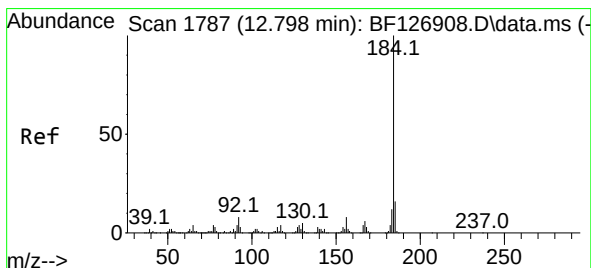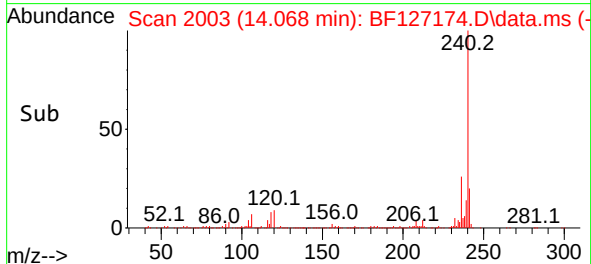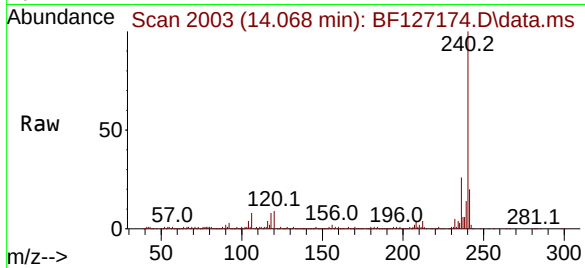

#77
Benzidine
Concen: 3.952 ng
RT: 13.010 min Scan# 1823
Delta R.T. 0.247 min
Lab File: BF127174.D
Acq: 03 Mar 2022 16:39

Tgt Ion:184 Resp: 16327
Ion Ratio Lower Upper
184 100
185 18.0 11.8 17.8#
183 6.3 8.2 12.2#


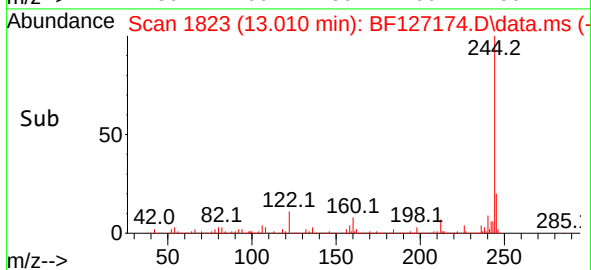

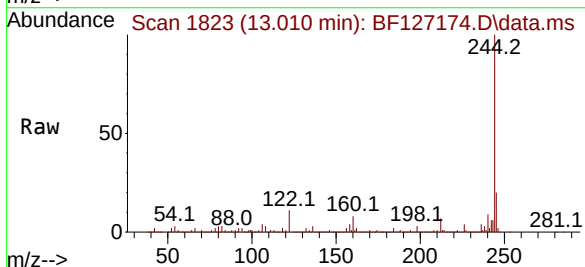


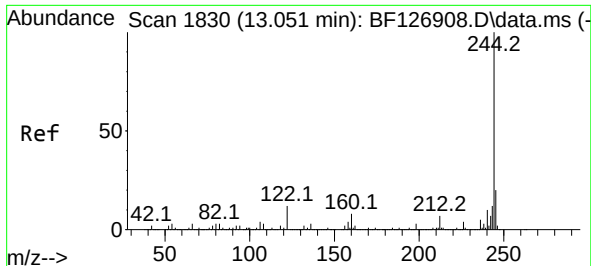

#79
 Terphenyl-d14
 Concen: 103.296 ng
 RT: 13.010 min Scan# 1823
 Delta R.T. -0.006 min
 Lab File: BF127174.D
 Acq: 03 Mar 2022 16:39

Instrument :
 BNA_F
 ClientSampleId :
 MW-40

Tgt Ion:244 Resp: 1068141
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.0 7.4
 122 11.2 13.3 19.9#

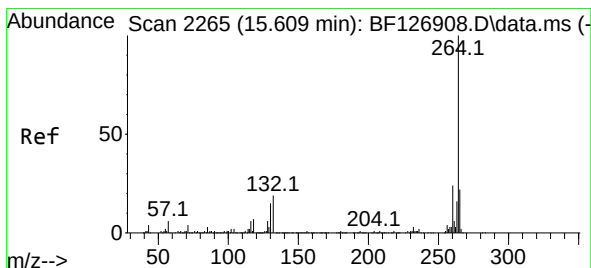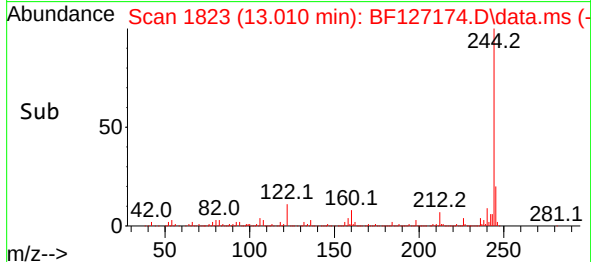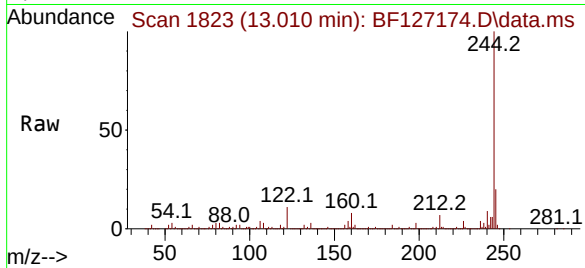

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.556 min Scan# 2256
 Delta R.T. -0.012 min
 Lab File: BF127174.D
 Acq: 03 Mar 2022 16:39

Tgt Ion:264 Resp: 147838
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.2 28.8
 265 21.2 17.4 26.2

