
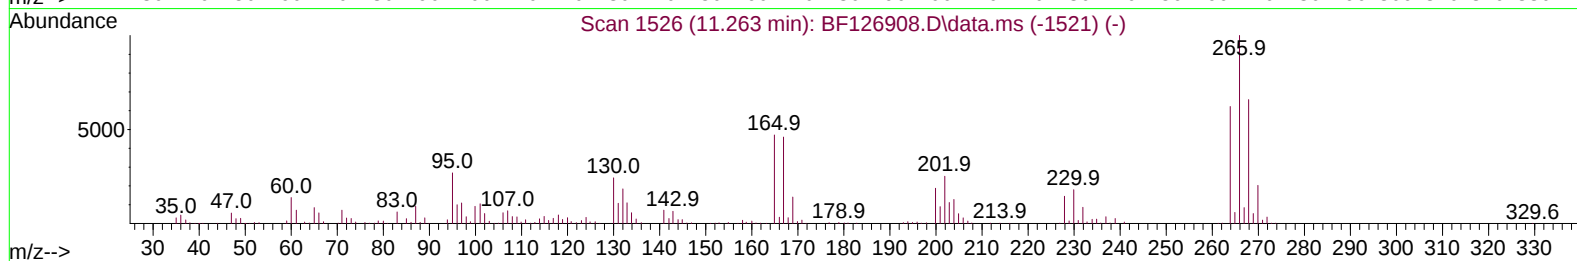
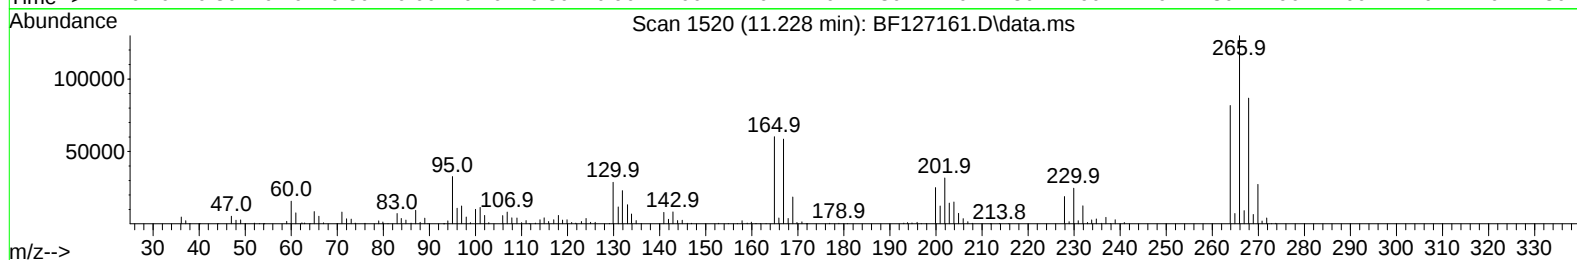


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
 Data File : BF127161.D
 Acq On : 03 Mar 2022 09:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 16:53:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 01 23:57:09 2022
 Response via : Initial Calibration

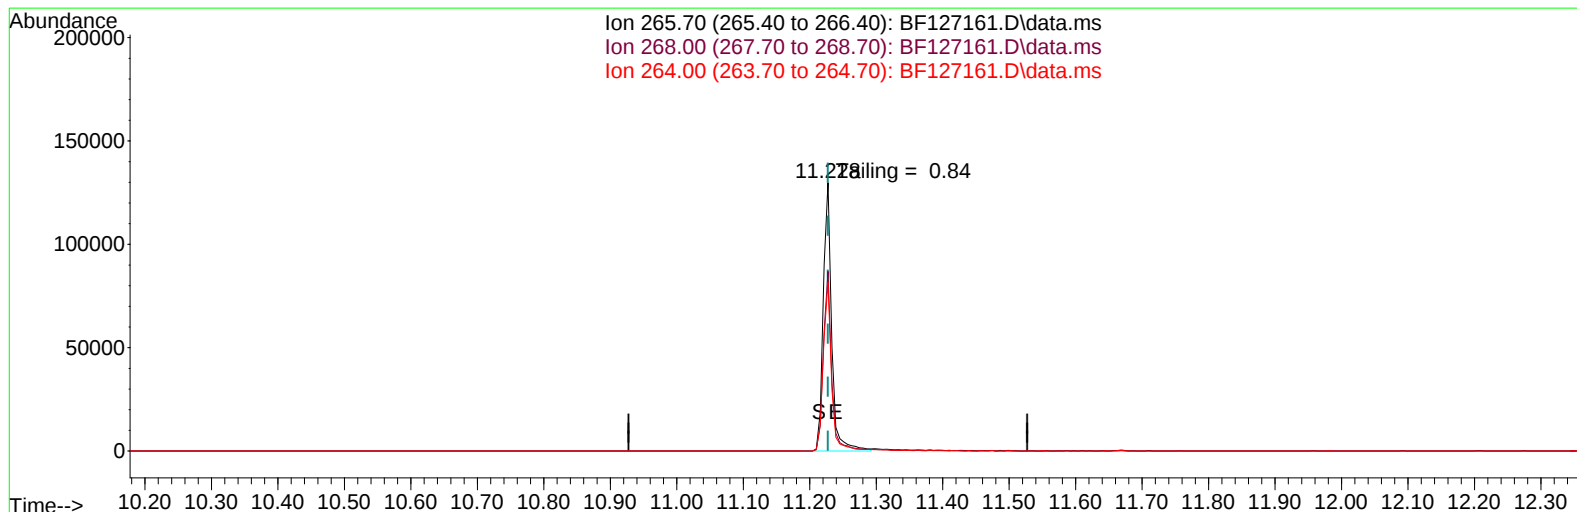

TIC: BF127161.D\data.ms

(70) Pentachlorophenol (C)




11.228min (+ 0.000) 23716.25 ng

response 117413

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.89
264.00	63.00	62.91
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\  
Data File : BF127161.D  
Acq On    : 03 Mar 2022  09:49  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 03 16:53:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 01 23:57:09 2022
Response via : Initial Calibration

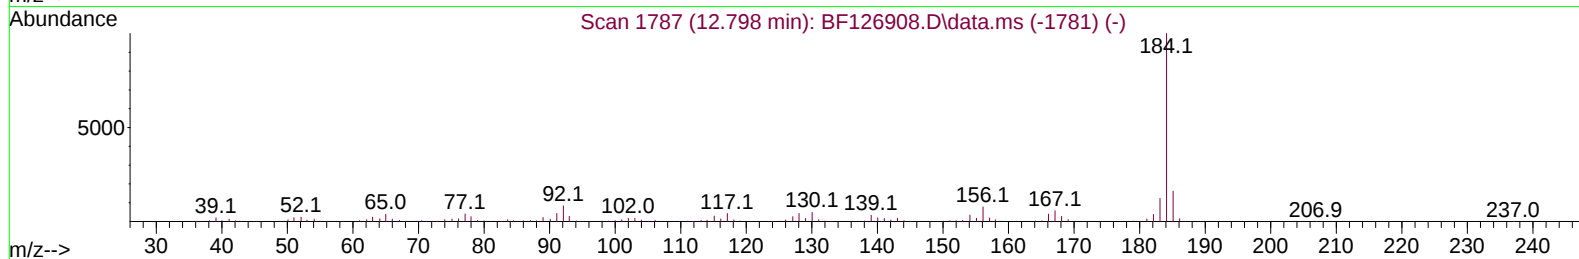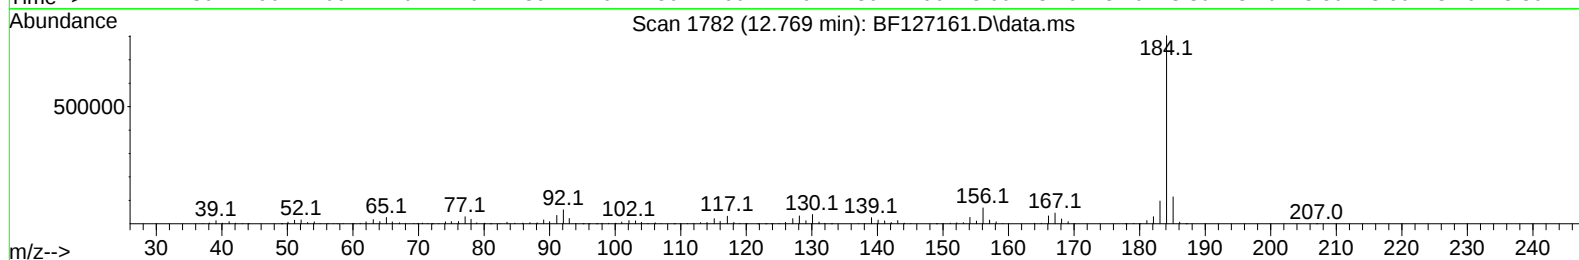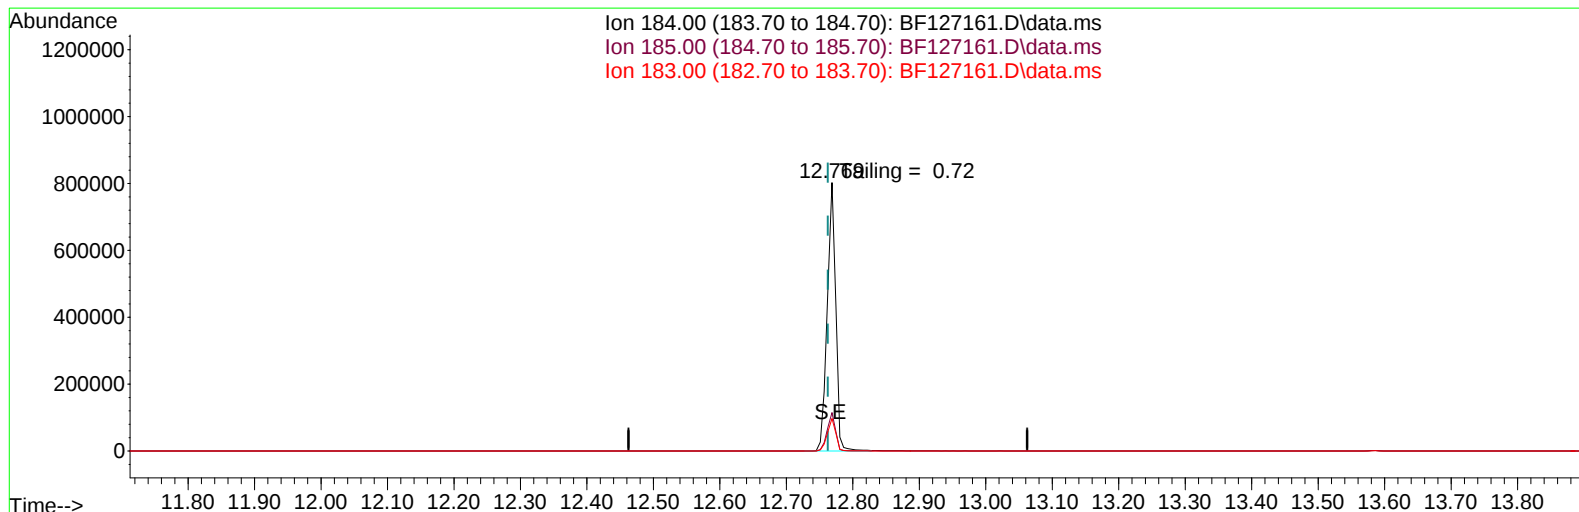

TIC: BF127161.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 314189.40 ng

response 717218

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.35
183.00	10.20	12.14
0.00	0.00	0.00