
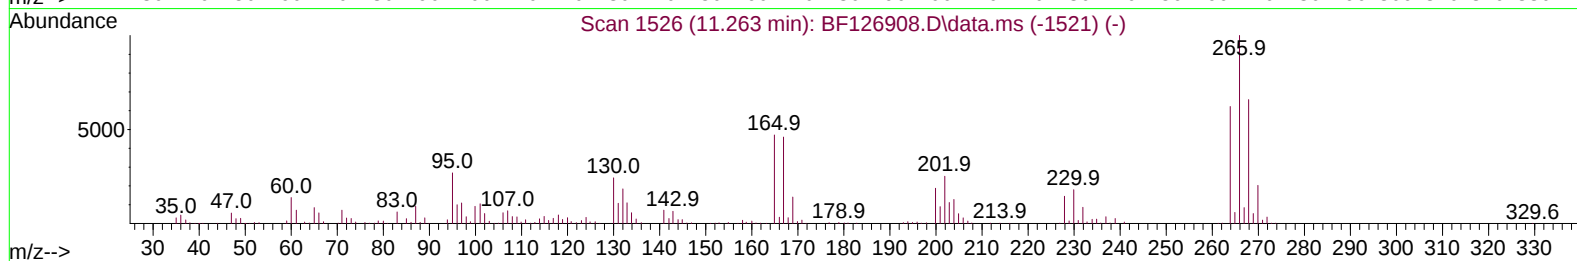
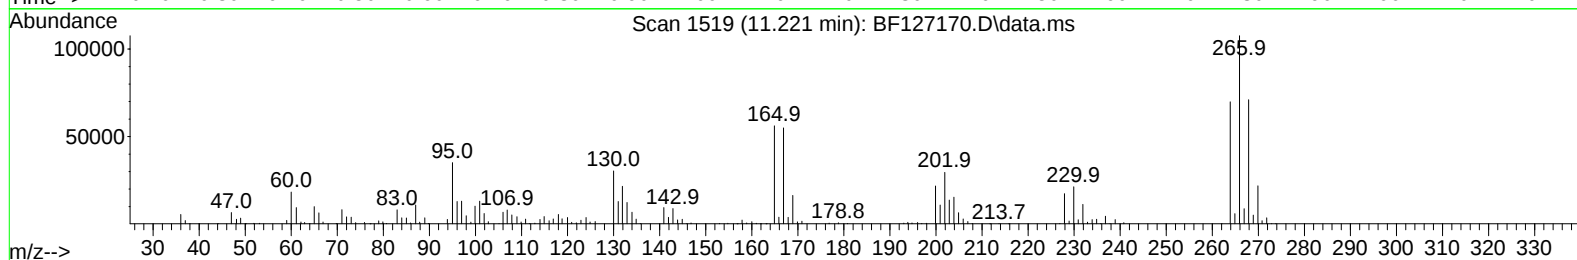


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127170.D
Acq On : 03 Mar 2022 14:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 17:15:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 01 23:57:09 2022
Response via : Initial Calibration

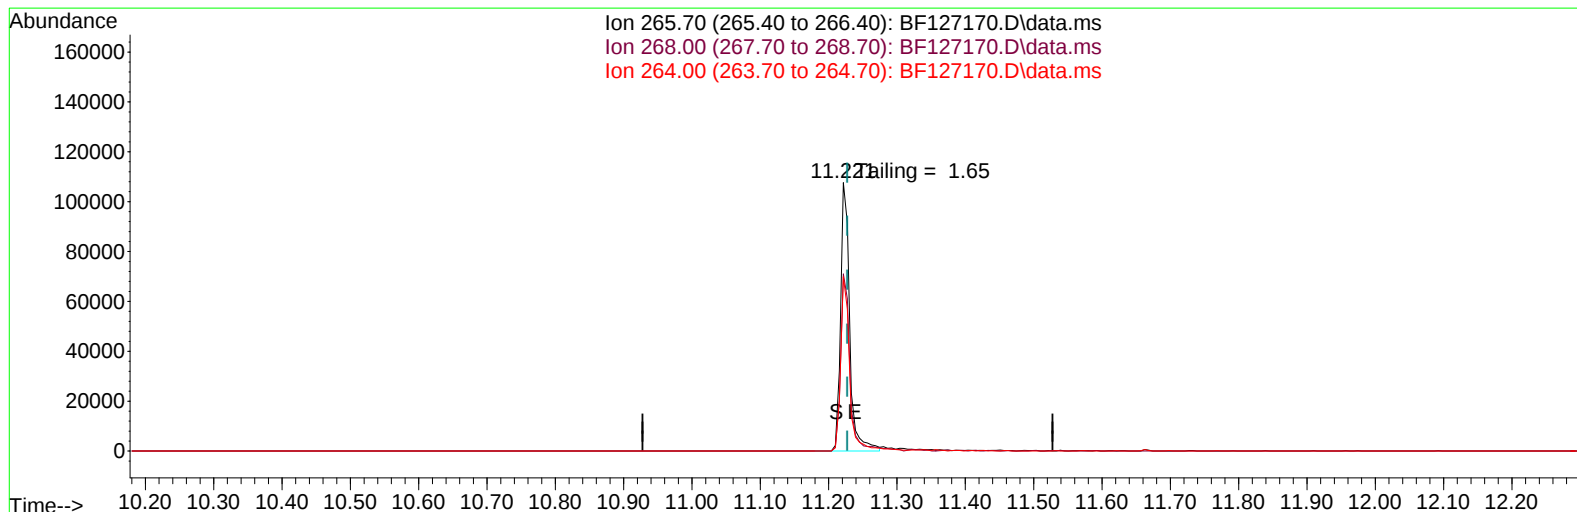

TIC: BF127170.D\data.ms

(70) Pentachlorophenol (C)




11.221min (-0.006) 253275.65 ng

response 101443

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.01
264.00	63.00	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
 Data File : BF127170.D
 Acq On : 03 Mar 2022 14:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 17:15:29 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 01 23:57:09 2022
 Response via : Initial Calibration

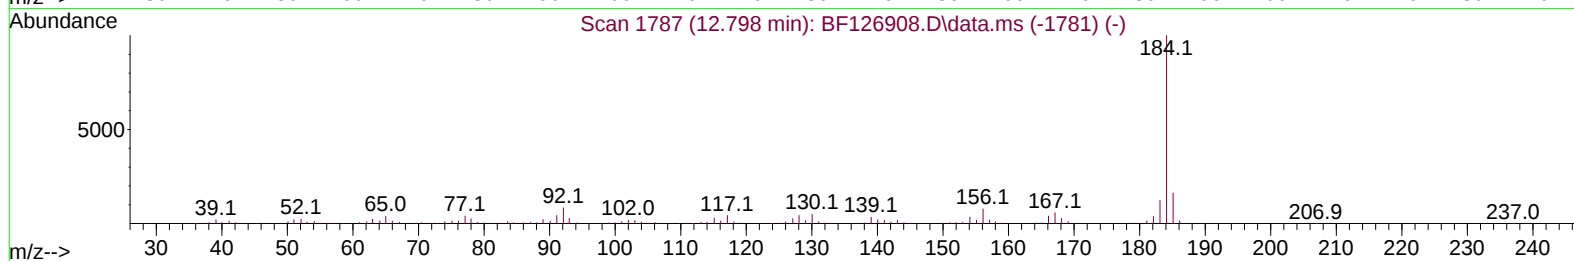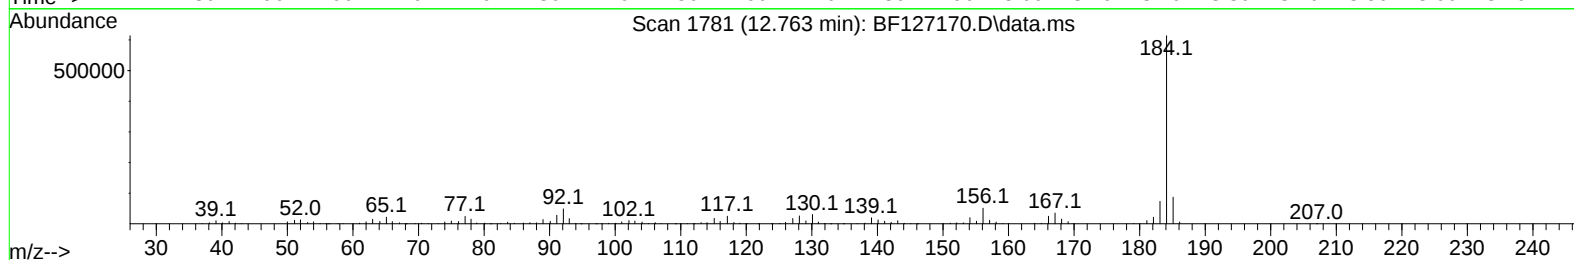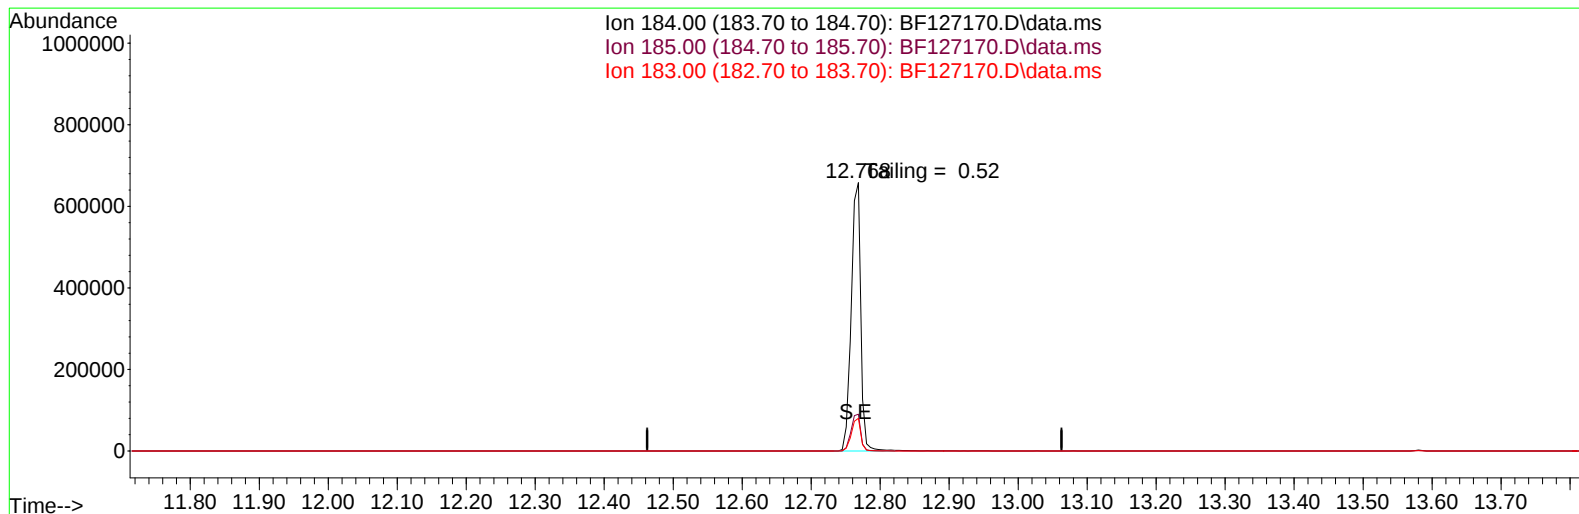

TIC: BF127170.D\data.ms

(77) Benzidine

12.763min (-12.763) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.80	0.00#
183.00	10.20	0.00#
0.00	0.00	0.00