

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF030322\  
 Data File : BF127163.D  
 Acq On : 03 Mar 2022 10:45  
 Operator : CG\JU  
 Sample : PB143032BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB143032BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF021622.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127163.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.522       | 545           | 550         | 553          | rBV      | 3429659        | 3224537       | 72.16%          | 12.892%       |
| 2         | 6.522       | 715           | 720         | 723          | rBV      | 2975875        | 3286666       | 73.55%          | 13.141%       |
| 3         | 6.886       | 779           | 782         | 786          | rBV      | 792432         | 665116        | 14.88%          | 2.659%        |
| 4         | 7.457       | 873           | 879         | 882          | rBV      | 2278591        | 2250203       | 50.35%          | 8.997%        |
| 5         | 8.175       | 996           | 1001        | 1004         | rBV      | 941047         | 908572        | 20.33%          | 3.633%        |
| 6         | 9.251       | 1178          | 1184        | 1187         | rBV      | 4323742        | 3939855       | 88.16%          | 15.752%       |
| 7         | 9.933       | 1295          | 1300        | 1303         | rBV      | 1108871        | 1004345       | 22.47%          | 4.015%        |
| 8         | 10.727      | 1430          | 1435        | 1438         | rBV      | 2850943        | 2638860       | 59.05%          | 10.550%       |
| 9         | 11.421      | 1549          | 1553        | 1557         | rBV      | 1304198        | 1061875       | 23.76%          | 4.246%        |
| 10        | 13.015      | 1818          | 1824        | 1827         | rBV      | 4743221        | 4468764       | 100.00%         | 17.867%       |
| 11        | 14.068      | 1999          | 2003        | 2006         | rBV      | 988437         | 846615        | 18.95%          | 3.385%        |
| 12        | 15.562      | 2251          | 2257        | 2264         | rBV      | 495096         | 615109        | 13.76%          | 2.459%        |
| 13        | 16.009      | 2328          | 2333        | 2338         | rBV2     | 31144          | 48596         | 1.09%           | 0.194%        |
| 14        | 17.350      | 2554          | 2561        | 2562         | rBV6     | 29750          | 52594         | 1.18%           | 0.210%        |




Sum of corrected areas: 25011707

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF030322\  
Data File : BF127163.D  
Acq On : 03 Mar 2022 10:45  
Operator : CG\JU  
Sample : PB143032BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB143032BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF021622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

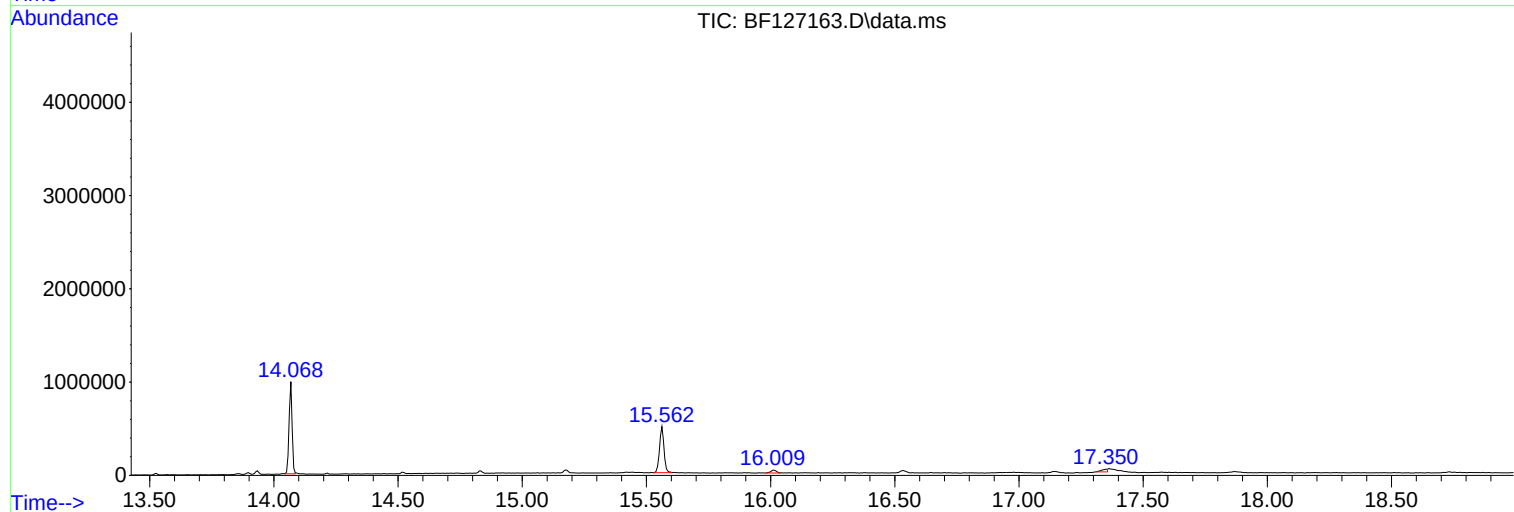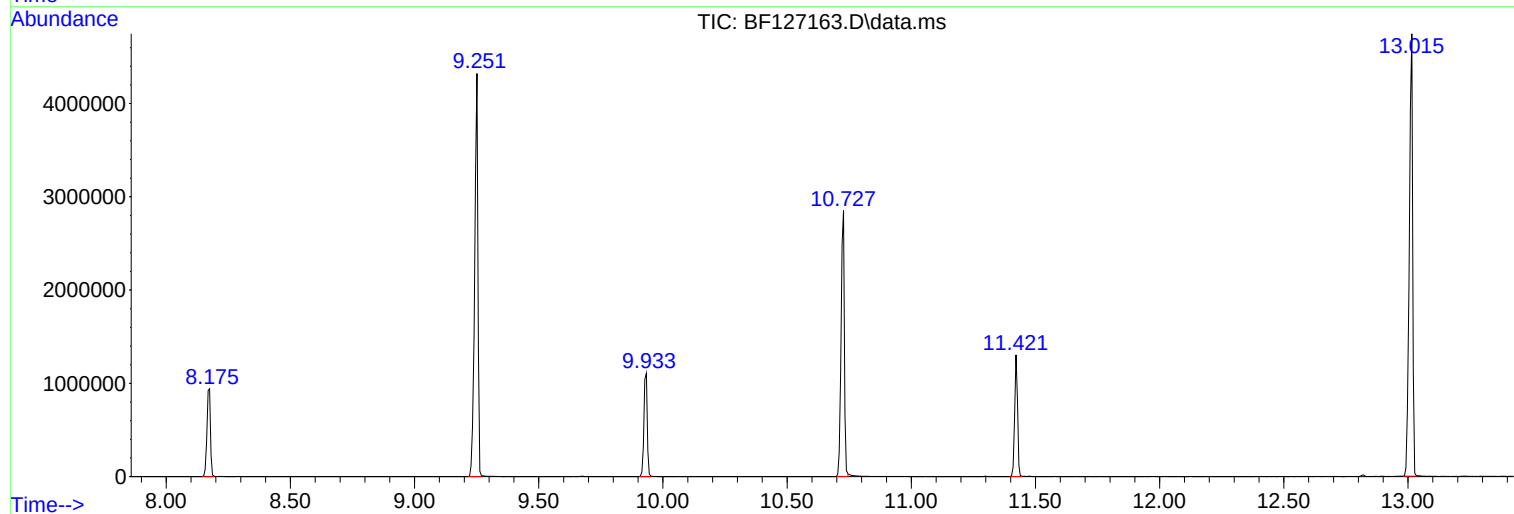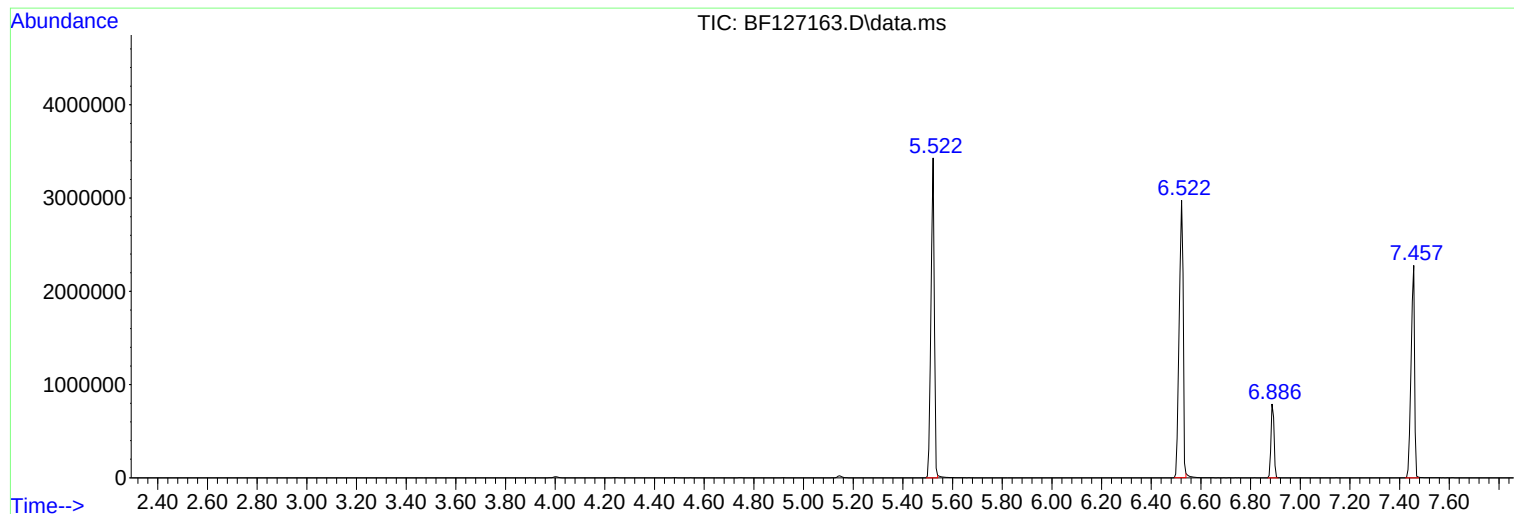

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF030322\  
Data File : BF127163.D  
Acq On : 03 Mar 2022 10:45  
Operator : CG\JU  
Sample : PB143032BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB143032BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF021622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF030322\  
Data File : BF127163.D  
Acq On : 03 Mar 2022 10:45  
Operator : CG\JU  
Sample : PB143032BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB143032BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF021622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|