

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
 Data File : BF127166.D
 Acq On : 03 Mar 2022 12:41
 Operator : CG\JU
 Sample : PB143042BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143042BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127166.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	545	550	553	rBV	2915657	2762205	72.23%	12.928%
2	6.522	714	720	723	rBV	2647714	2799489	73.20%	13.103%
3	6.887	779	782	786	rBV	695719	564074	14.75%	2.640%
4	7.457	873	879	882	rBV	1874783	1902676	49.75%	8.905%
5	8.169	996	1000	1004	rBV	809738	750126	19.61%	3.511%
6	9.251	1178	1184	1187	rBV	3831628	3389575	88.63%	15.865%
7	9.928	1295	1299	1303	rBV	932406	813937	21.28%	3.810%
8	10.722	1430	1434	1438	rBV	2255310	2241801	58.62%	10.493%
9	11.422	1549	1553	1556	rBV	1093913	874731	22.87%	4.094%
10	13.016	1818	1824	1826	rBV	3753390	3824362	100.00%	17.900%
11	13.933	1976	1980	1984	rVB	43742	45326	1.19%	0.212%
12	14.069	1999	2003	2006	rBV	741894	674906	17.65%	3.159%
13	15.174	2187	2191	2197	rVB	37818	43356	1.13%	0.203%
14	15.563	2251	2257	2267	rBV	457223	581208	15.20%	2.720%
15	16.010	2328	2333	2340	rVB2	32887	50203	1.31%	0.235%
16	16.527	2416	2421	2429	rBV2	25829	47726	1.25%	0.223%




Sum of corrected areas: 21365701

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127166.D
Acq On : 03 Mar 2022 12:41
Operator : CG\JU
Sample : PB143042BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143042BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

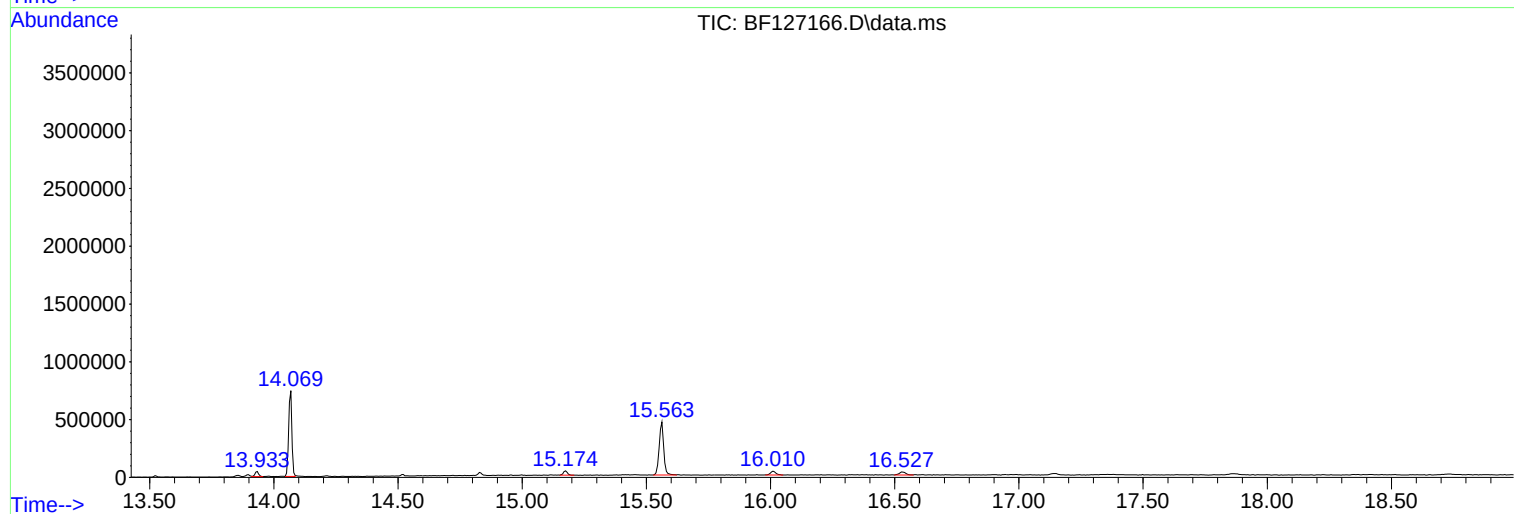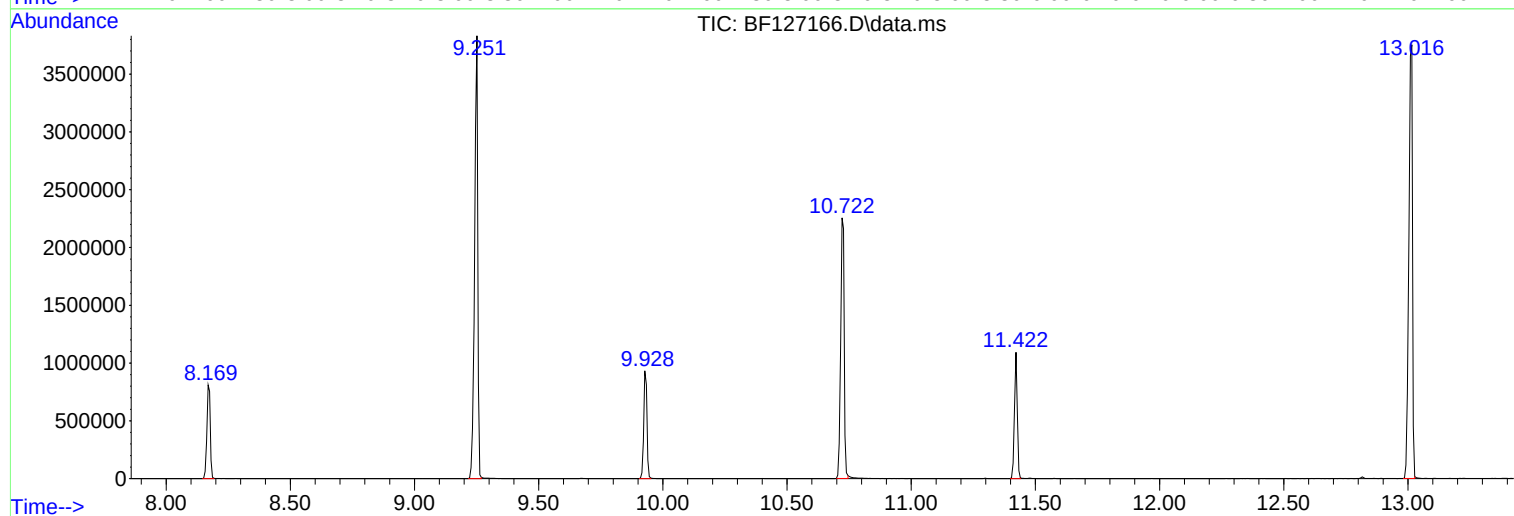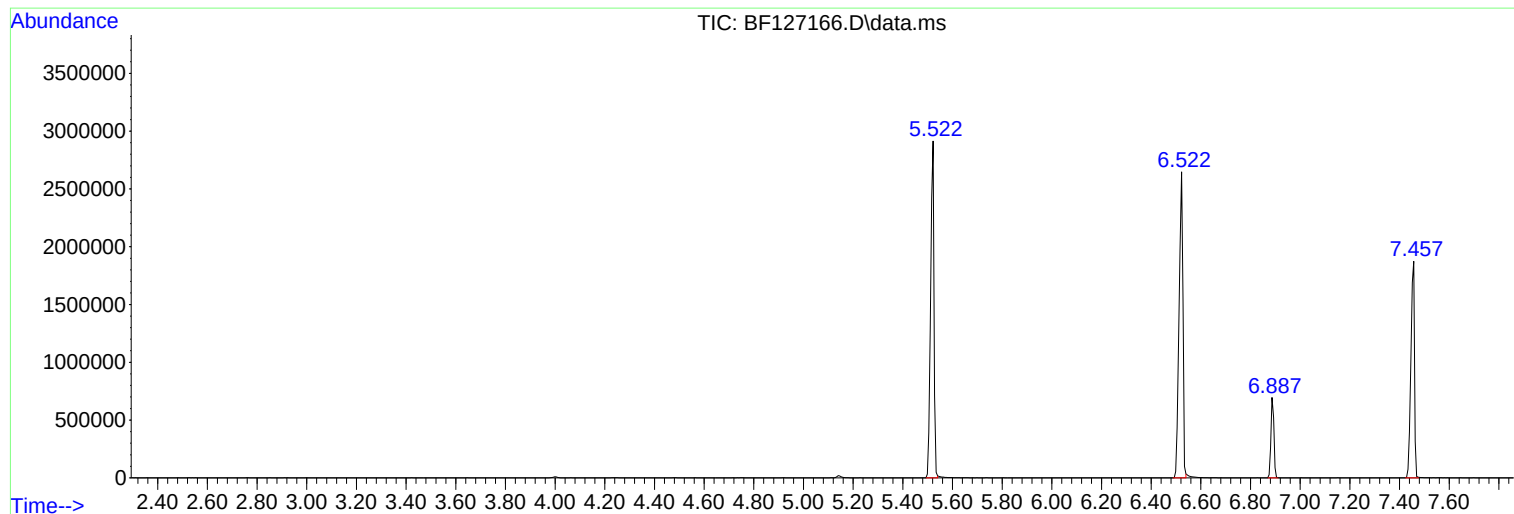

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127166.D
Acq On : 03 Mar 2022 12:41
Operator : CG\JU
Sample : PB143042BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143042BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127166.D
Acq On : 03 Mar 2022 12:41
Operator : CG\JU
Sample : PB143042BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143042BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------