

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
 Data File : BF127169.D
 Acq On : 03 Mar 2022 14:08
 Operator : CG\JU
 Sample : PB143033BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143033BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.522	545	550	553	rBV	3220132	3227135	83.73%	13.537%
2	6.522	715	720	723	rBV	3075807	3229659	83.80%	13.548%
3	6.886	779	782	786	rBV	835288	672417	17.45%	2.821%
4	7.457	873	879	882	rBV	2194296	2242665	58.19%	9.408%
5	8.169	996	1000	1004	rBV	980966	902139	23.41%	3.784%
6	9.251	1178	1184	1187	rBV	4257769	3836132	99.53%	16.092%
7	9.927	1295	1299	1303	rBV	1044208	968945	25.14%	4.065%
8	10.722	1430	1434	1438	rBV	2591424	2527940	65.59%	10.604%
9	11.421	1549	1553	1556	rBV	1213806	975966	25.32%	4.094%
10	13.010	1818	1823	1826	rBV	3851724	3854140	100.00%	16.167%
11	13.933	1976	1980	1985	rVB	60962	61390	1.59%	0.258%
12	14.068	1999	2003	2006	rBV	778571	683296	17.73%	2.866%
13	15.562	2251	2257	2264	rBV2	406553	559721	14.52%	2.348%
14	16.009	2329	2333	2341	rVB	31226	50238	1.30%	0.211%
15	16.533	2416	2422	2430	rVB2	24709	47121	1.22%	0.198%




Sum of corrected areas: 23838904

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127169.D
Acq On : 03 Mar 2022 14:08
Operator : CG\JU
Sample : PB143033BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143033BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

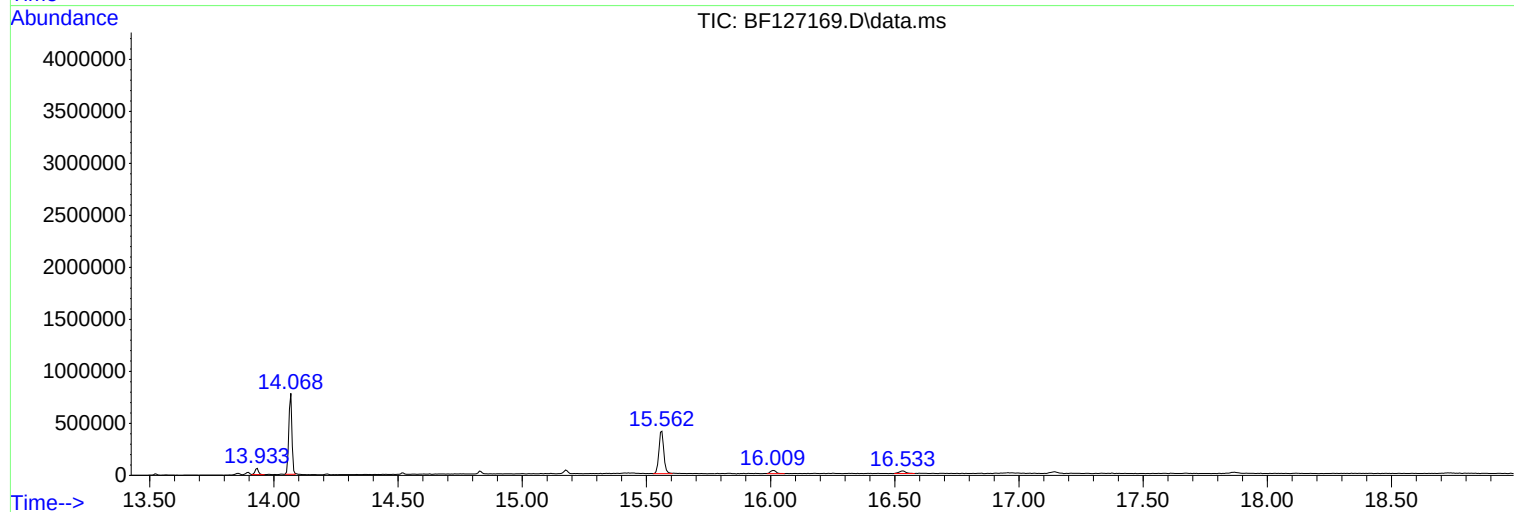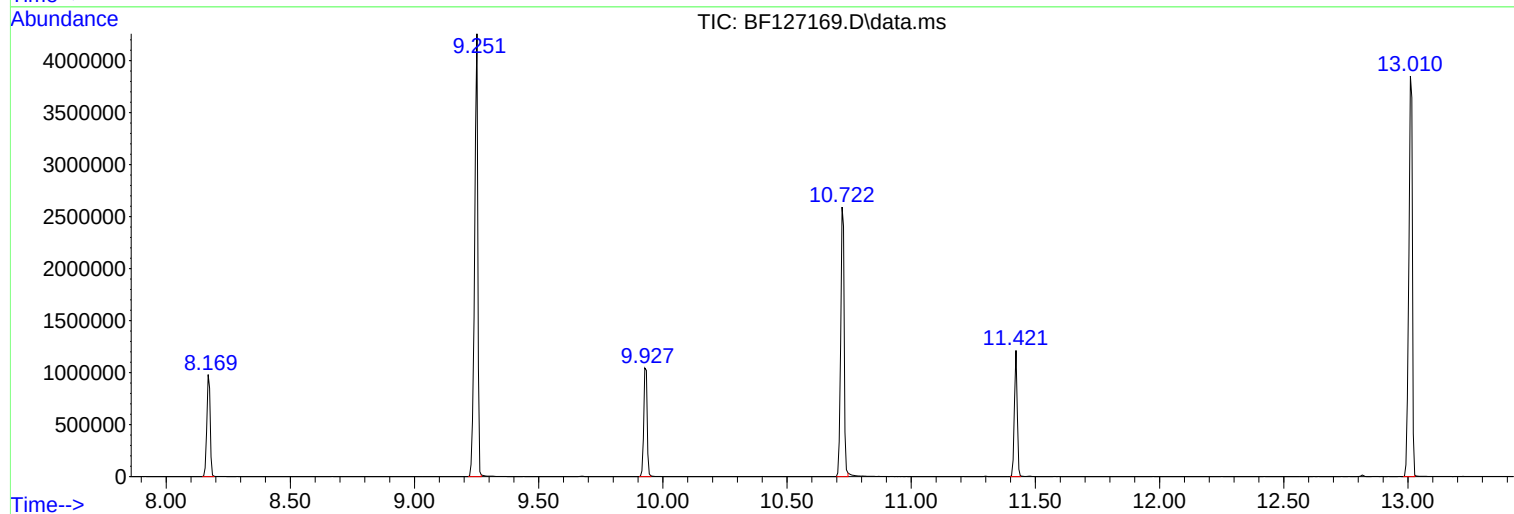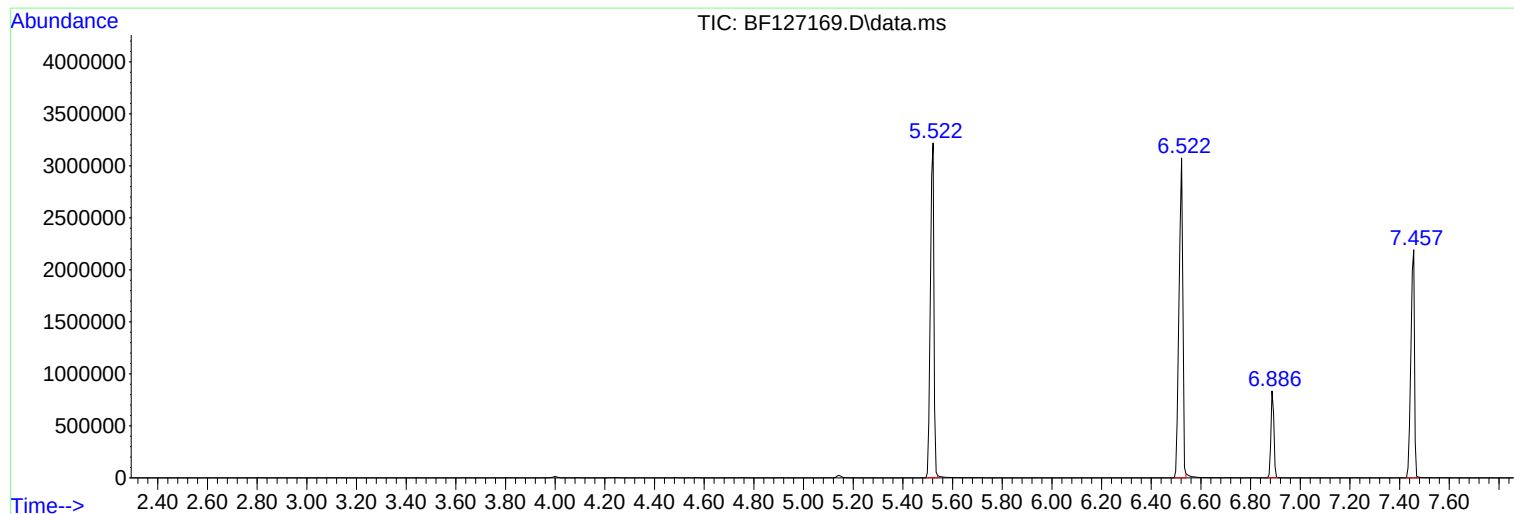

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127169.D
Acq On : 03 Mar 2022 14:08
Operator : CG\JU
Sample : PB143033BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143033BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127169.D
Acq On : 03 Mar 2022 14:08
Operator : CG\JU
Sample : PB143033BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143033BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------