

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
 Data File : BF127173.D
 Acq On : 03 Mar 2022 16:09
 Operator : CG\JU
 Sample : N1689-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-45

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	544	548	561	rBV	1298756	1149897	34.89%	6.824%
2	6.516	715	719	725	rBV	820447	723314	21.95%	4.293%
3	6.886	779	782	786	rBV	654333	519413	15.76%	3.082%
4	7.457	873	879	882	rBV	1913725	1858303	56.39%	11.028%
5	8.092	983	987	996	rBV3	19294	42383	1.29%	0.252%
6	8.169	996	1000	1004	rBV	785086	707561	21.47%	4.199%
7	9.251	1178	1184	1187	rBV	3711128	3295488	100.00%	19.557%
8	9.927	1296	1299	1303	rBV	866075	776079	23.55%	4.606%
9	10.327	1362	1367	1369	rBV	45151	52728	1.60%	0.313%
10	10.722	1430	1434	1438	rBV	2206666	2216000	67.24%	13.151%
11	11.363	1540	1543	1546	rVB	71590	53435	1.62%	0.317%
12	11.421	1549	1553	1556	rBV	1003388	792433	24.05%	4.703%
13	11.580	1576	1580	1586	rBV	58882	66394	2.01%	0.394%
14	11.933	1637	1640	1643	rBV	61145	57103	1.73%	0.339%
15	11.974	1644	1647	1650	rVB	65968	52956	1.61%	0.314%
16	12.092	1663	1667	1673	rBV8	22260	39106	1.19%	0.232%
17	12.186	1679	1683	1687	rBV7	39403	49095	1.49%	0.291%
18	12.910	1801	1806	1813	rBV5	30438	61259	1.86%	0.364%
19	13.010	1818	1823	1826	rBV	3343919	2933806	89.02%	17.411%
20	13.851	1962	1966	1969	rBV	40319	53597	1.63%	0.318%
21	13.892	1969	1973	1976	rVV	56608	67639	2.05%	0.401%
22	13.927	1976	1979	1982	rVV	190513	196933	5.98%	1.169%
23	13.974	1982	1987	1994	rVB7	34633	85592	2.60%	0.508%
24	14.068	1999	2003	2006	rBV	502342	450038	13.66%	2.671%
25	14.821	2127	2131	2135	rBV3	29851	48400	1.47%	0.287%
26	14.904	2142	2145	2150	rBV5	25799	40171	1.22%	0.238%
27	15.556	2251	2256	2263	rVB	361750	461499	14.00%	2.739%




Sum of corrected areas: 16850622

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127173.D
Acq On : 03 Mar 2022 16:09
Operator : CG\JU
Sample : N1689-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

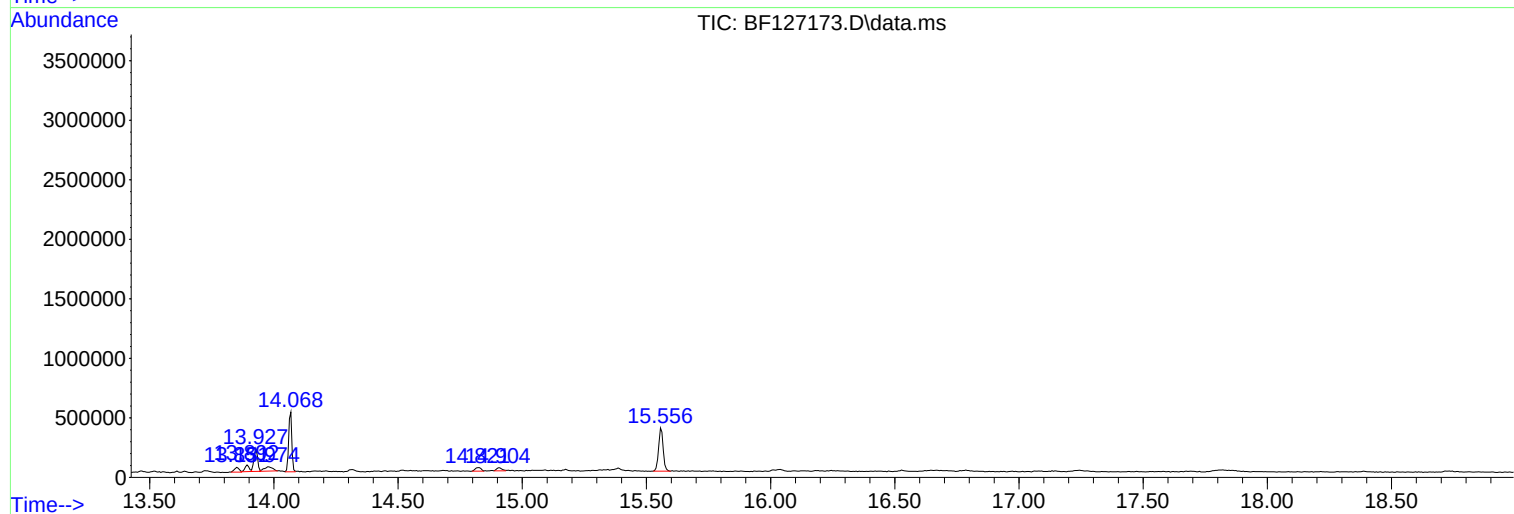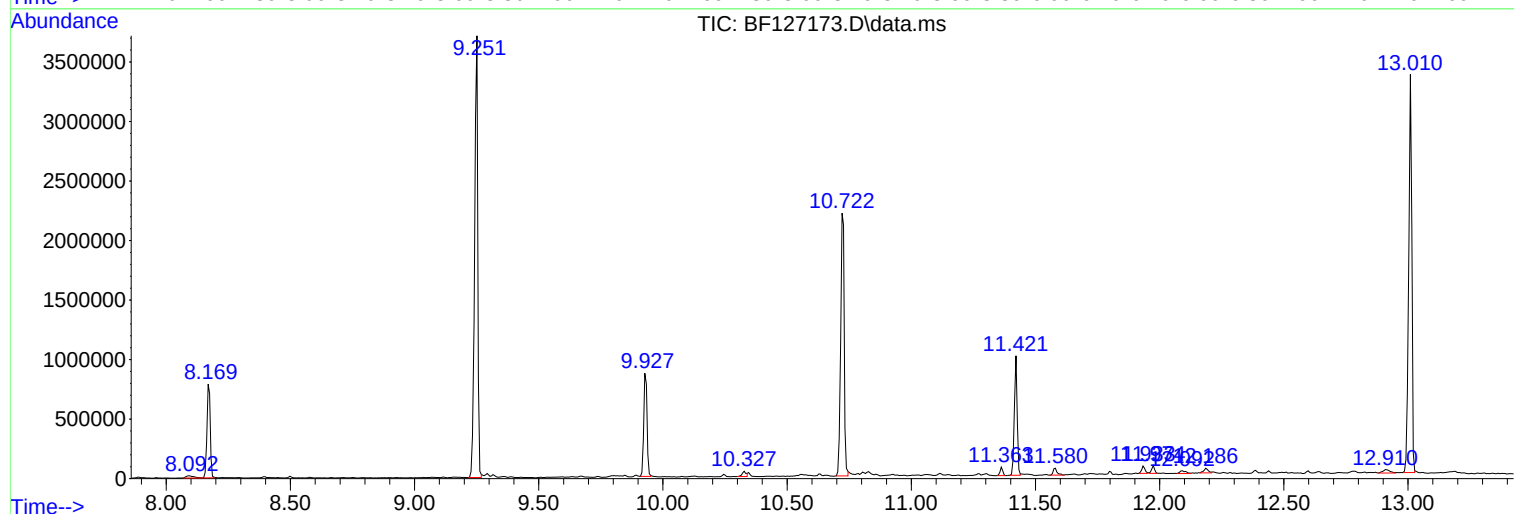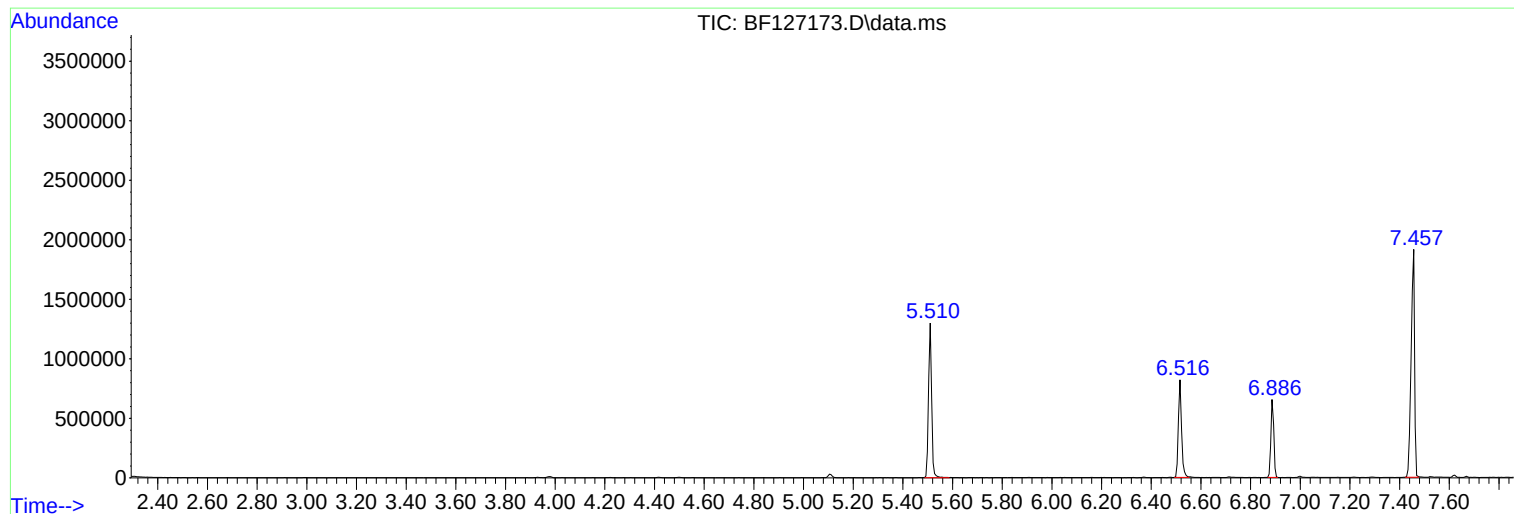

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127173.D
Acq On : 03 Mar 2022 16:09
Operator : CG\JU
Sample : N1689-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127173.D
Acq On : 03 Mar 2022 16:09
Operator : CG\JU
Sample : N1689-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-45

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------