
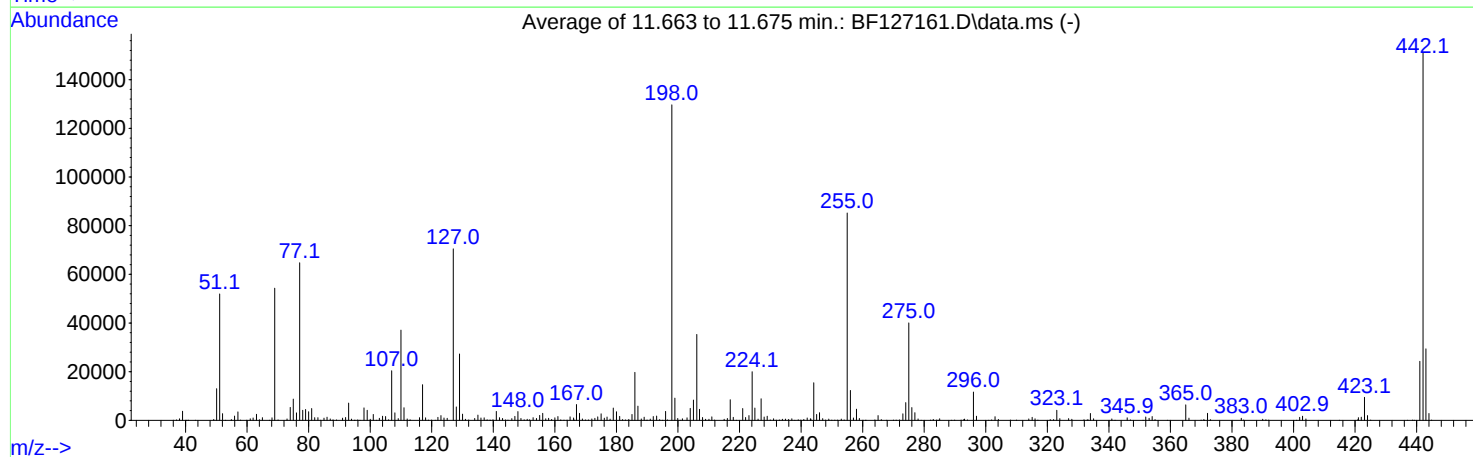


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
 Data File : BF127161.D
 Acq On : 03 Mar 2022 09:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 01 23:57:09 2022

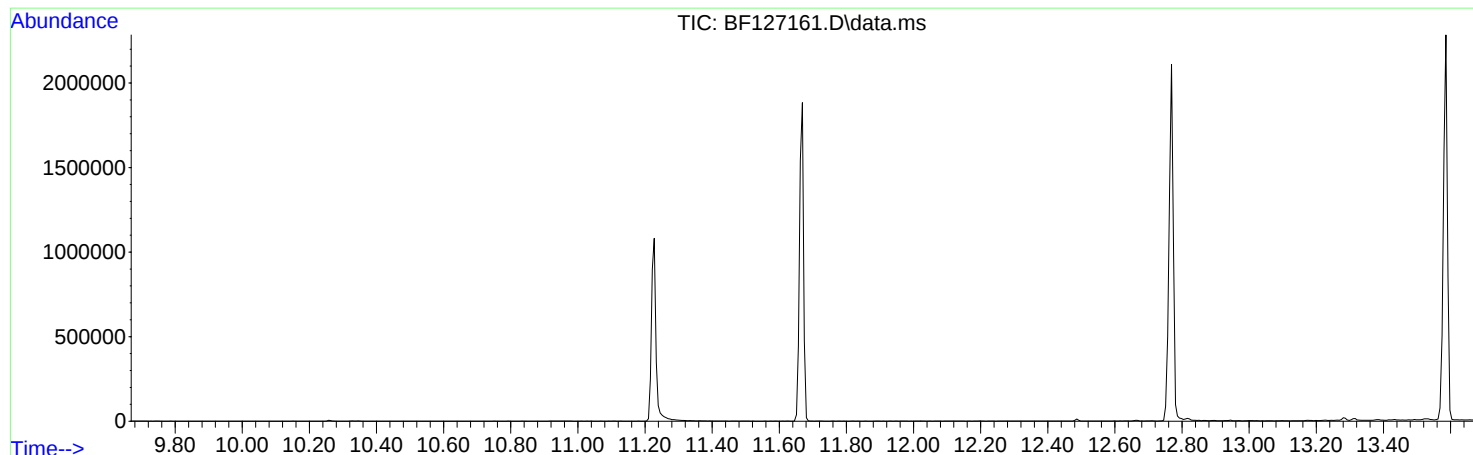




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	51969	PASS
68	69	0.00	2	2.0	1085	PASS
69	198	0.00	100	41.9	54313	PASS
70	69	0.00	2	0.4	237	PASS
127	198	10	80	54.4	70482	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	129664	PASS
199	198	5	9	7.0	9125	PASS
275	198	10	60	30.9	40040	PASS
365	198	1	100	4.9	6371	PASS
441	198	0.01	100	18.7	24253	PASS
442	442	50	100	100.0	151160	PASS
443	442	15	24	19.5	29419	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
 Data File : BF127161.D
 Acq On : 03 Mar 2022 09:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 03 16:53:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 01 23:57:09 2022
 Response via : Initial Calibration

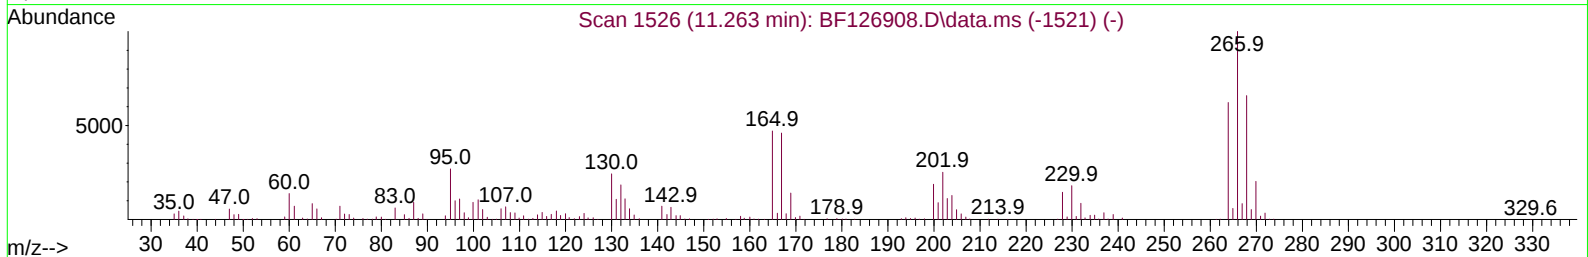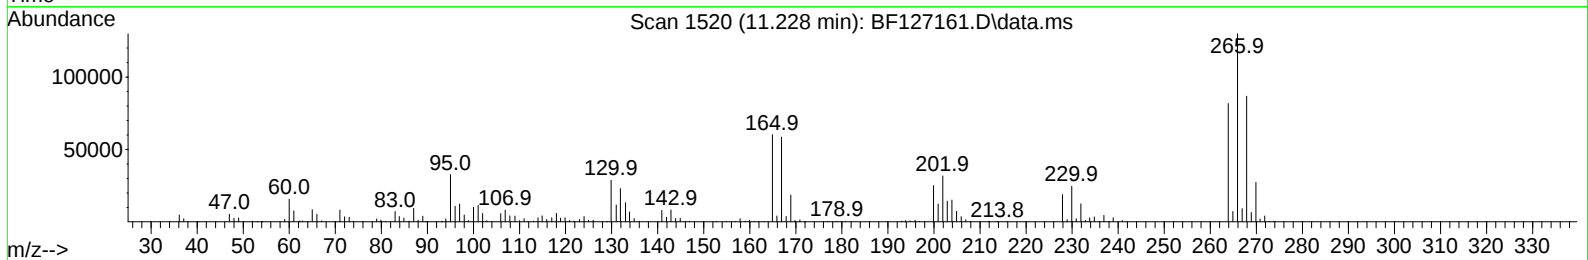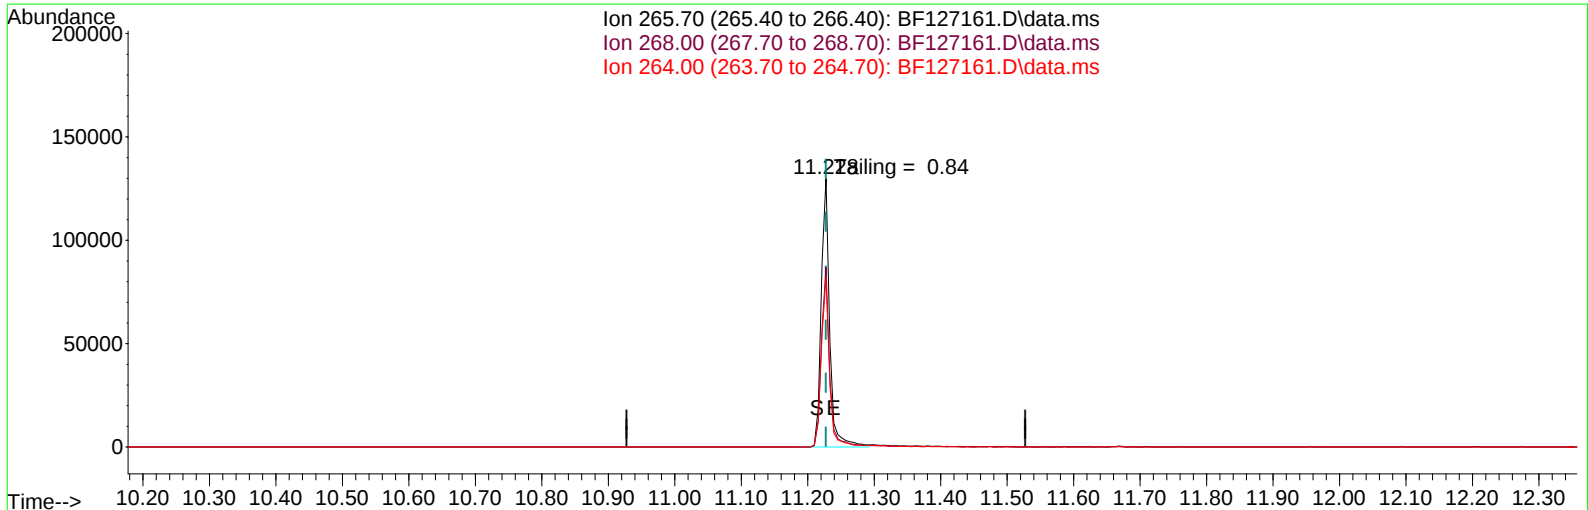

TIC: BF127161.D\data.ms

(70) Pentachlorophenol (C)

11.228min (+ 0.000) 23716.25 ng




response 117413

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.89
264.00	63.00	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
 Data File : BF127161.D
 Acq On : 03 Mar 2022 09:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 03 16:53:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 01 23:57:09 2022
 Response via : Initial Calibration

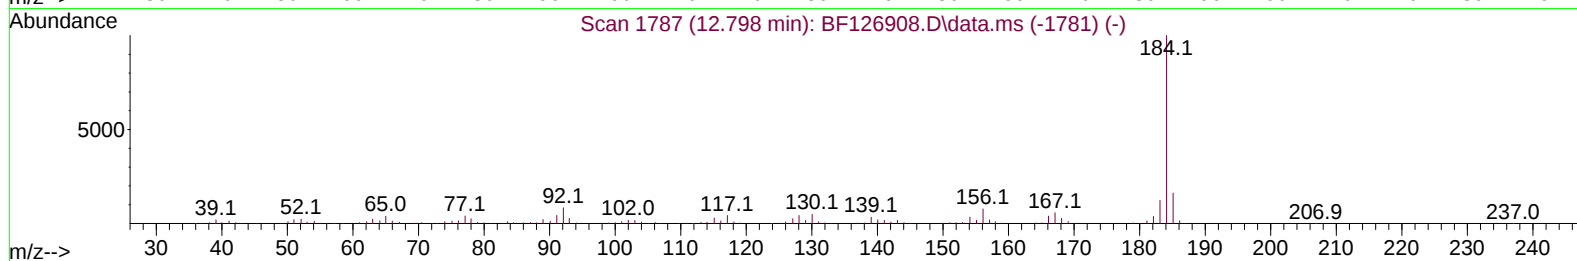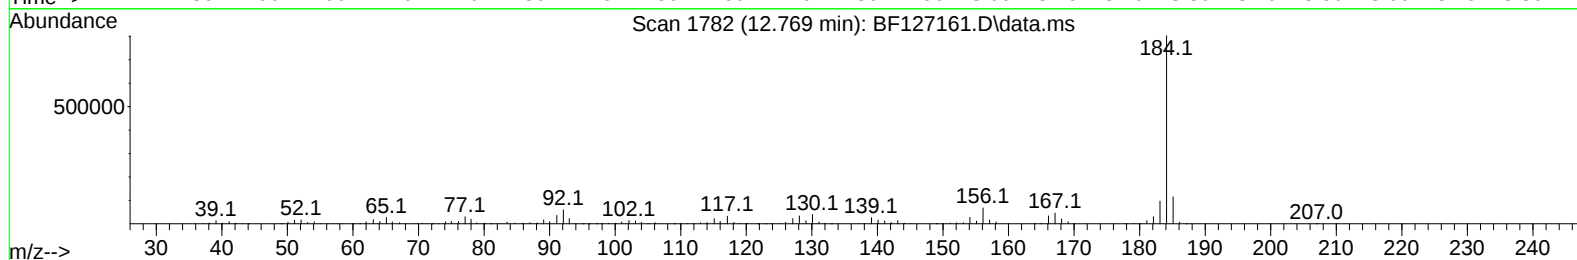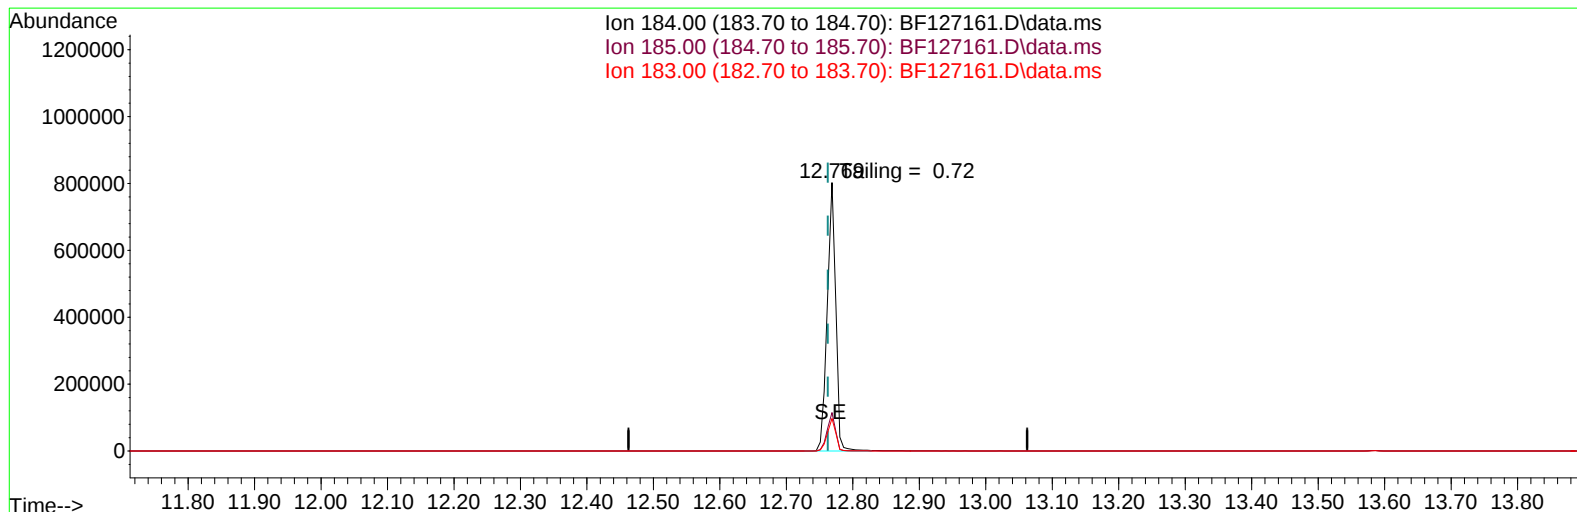

TIC: BF127161.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 314189.40 ng

response 717218

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.35
183.00	10.20	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/3/2022	BNA_F	<u>BF127161.D</u>
Compound Name	Response	Retention Time
DDT	344362	13.58
DDD	2613	13.28
DDE	0	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2613	346975	0.75

Instrument :
BNA_F
ClientSampleId :
DFTPP