


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
 Data File : BF127170.D
 Acq On : 03 Mar 2022 14:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 01 23:57:09 2022

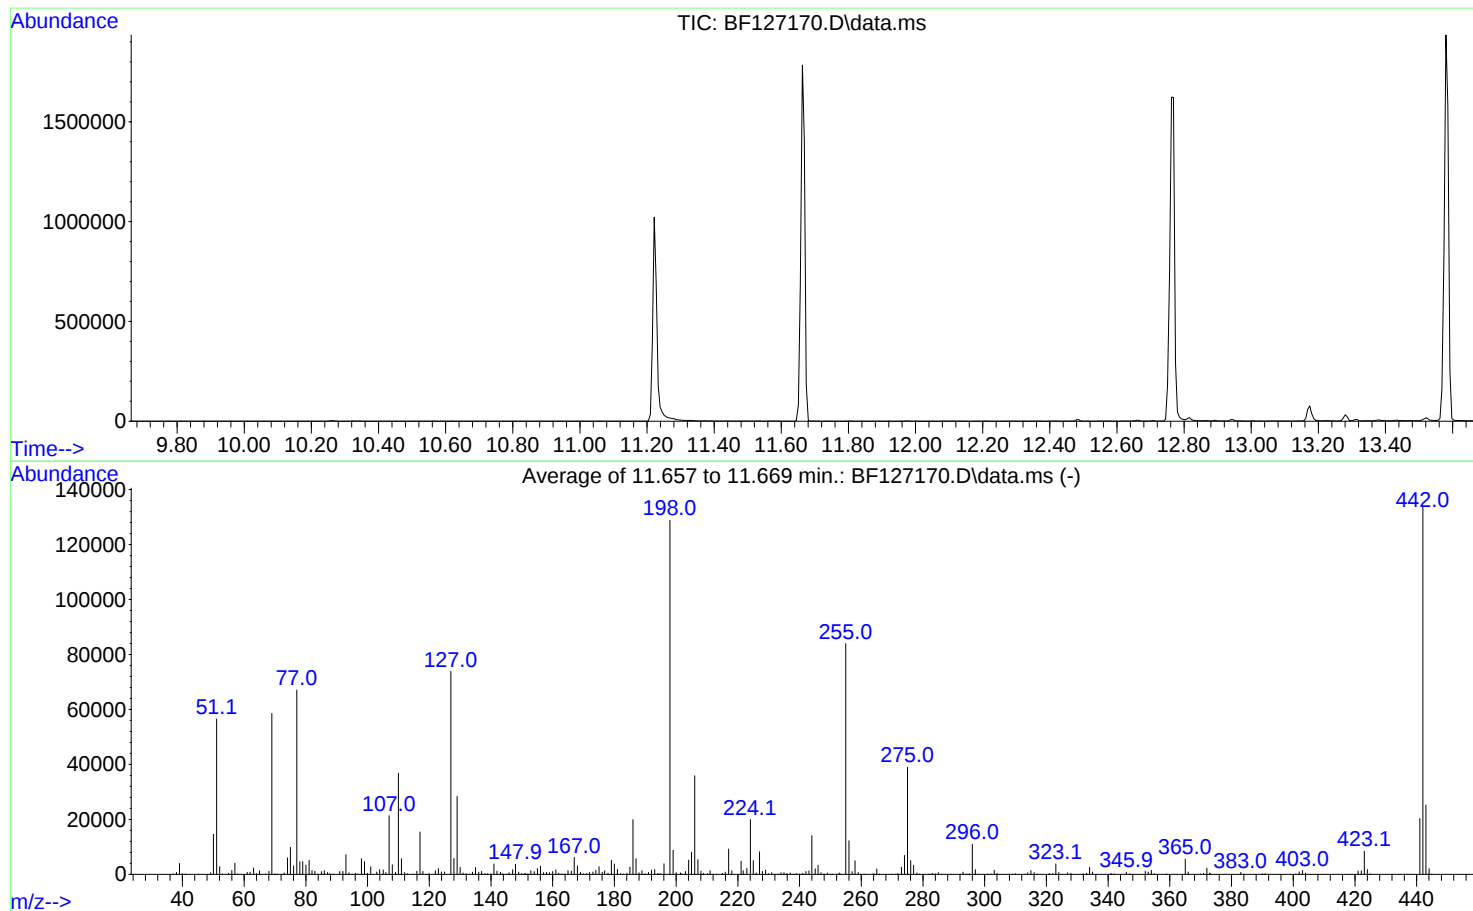




AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	56520	PASS
68	69	0.00	2	1.9	1093	PASS
69	198	0.00	100	45.5	58592	PASS
70	69	0.00	2	0.3	174	PASS
127	198	10	80	57.3	73872	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	128848	PASS
199	198	5	9	6.8	8810	PASS
275	198	10	60	30.3	39024	PASS
365	198	1	100	4.3	5527	PASS
441	198	0.01	100	15.8	20310	PASS
442	442	50	100	100.0	133853	PASS
443	442	15	24	18.8	25184	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127170.D
Acq On : 03 Mar 2022 14:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 03 17:15:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 01 23:57:09 2022
Response via : Initial Calibration

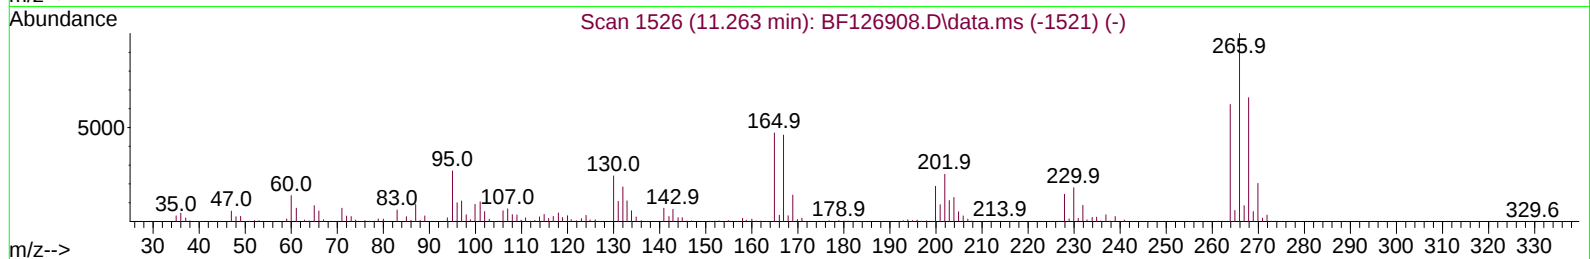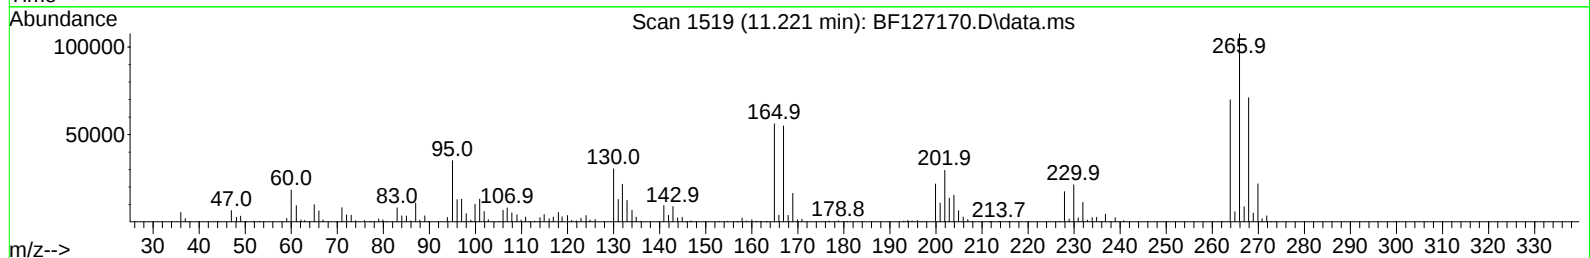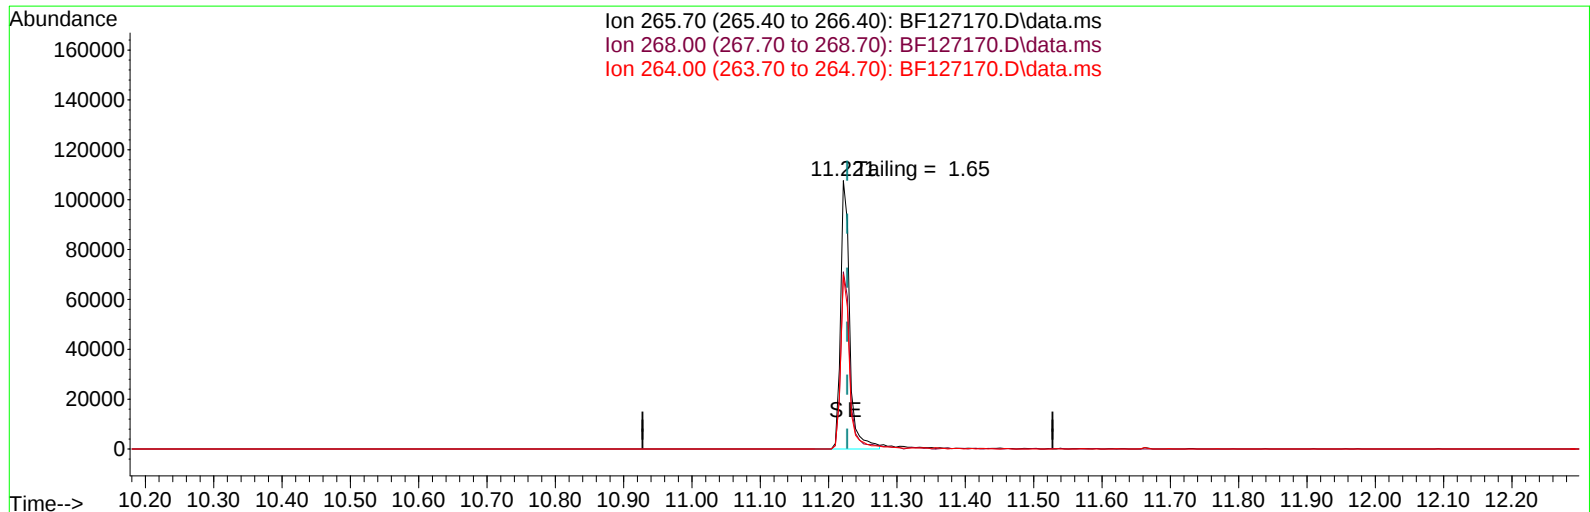

TIC: BF127170.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.006) 253275.65 ng




response 101443

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.01
264.00	63.00	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030322\
Data File : BF127170.D
Acq On : 03 Mar 2022 14:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 03 17:15:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 01 23:57:09 2022
Response via : Initial Calibration

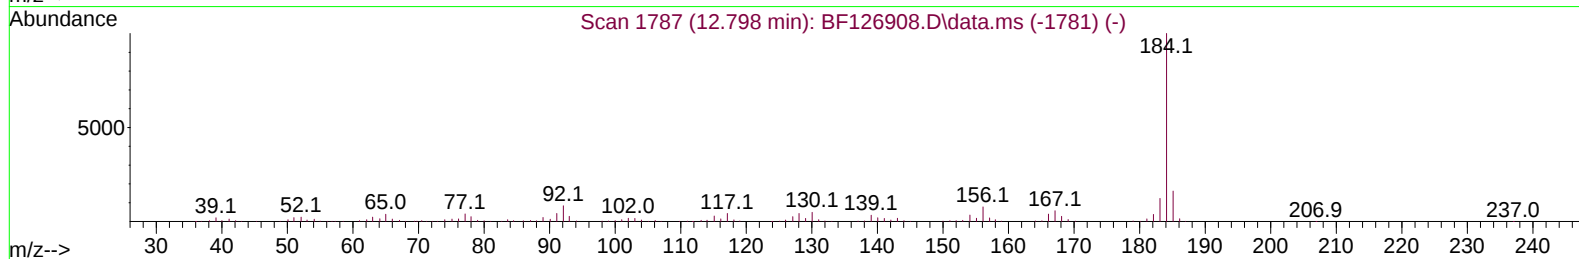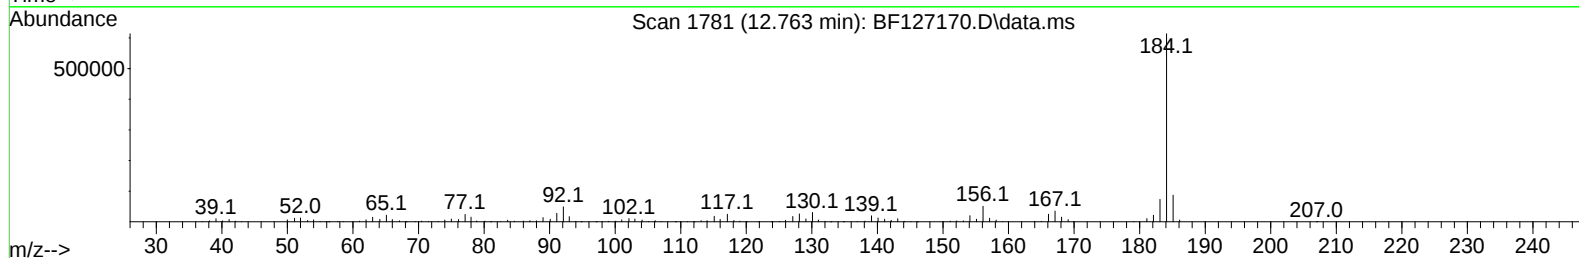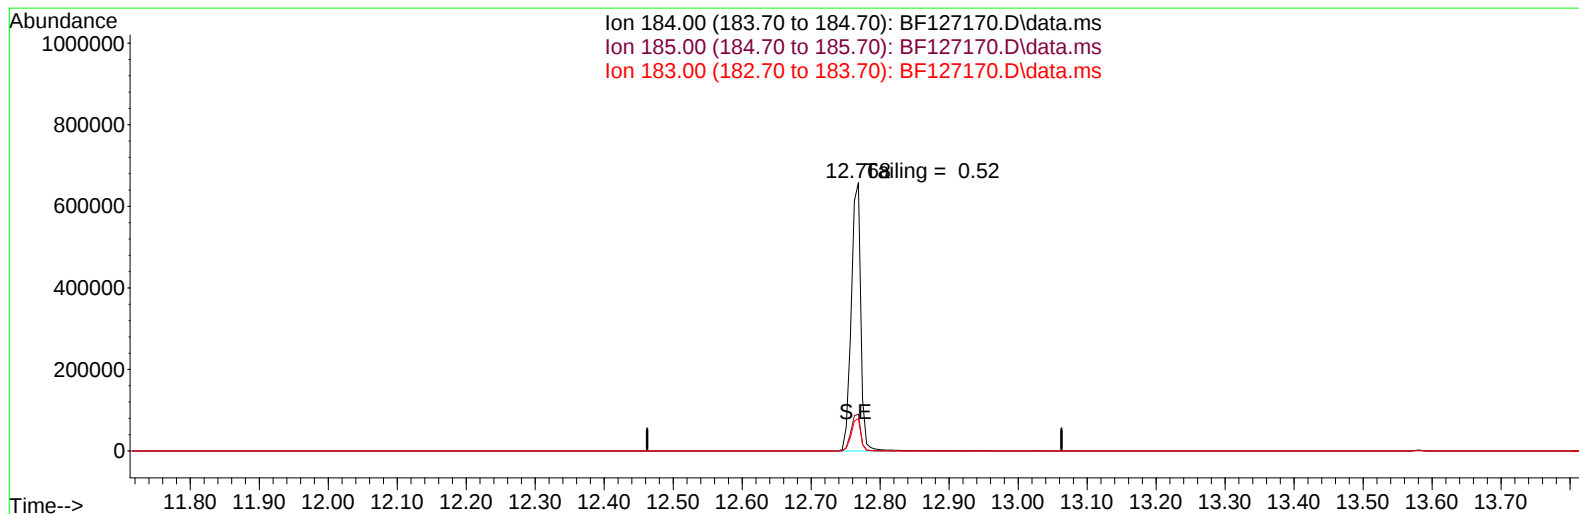

TIC: BF127170.D\data.ms

(77) Benzidine

12.763min (-12.763) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.80	0.00#
183.00	10.20	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/3/2022	BNA_F	<u>BF127170.D</u>
Compound Name	Response	Retention Time
DDT	306374	13.58
DDD	5199	13.28
DDE	1381	12.94
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6580	312954	2.10

Instrument :
BNA_F
ClientSampleId :
DFTPP