


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030415\
 Data File : BF077579.D
 Acq On : 4 Mar 2015 12:18
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 04 13:27:09 2015

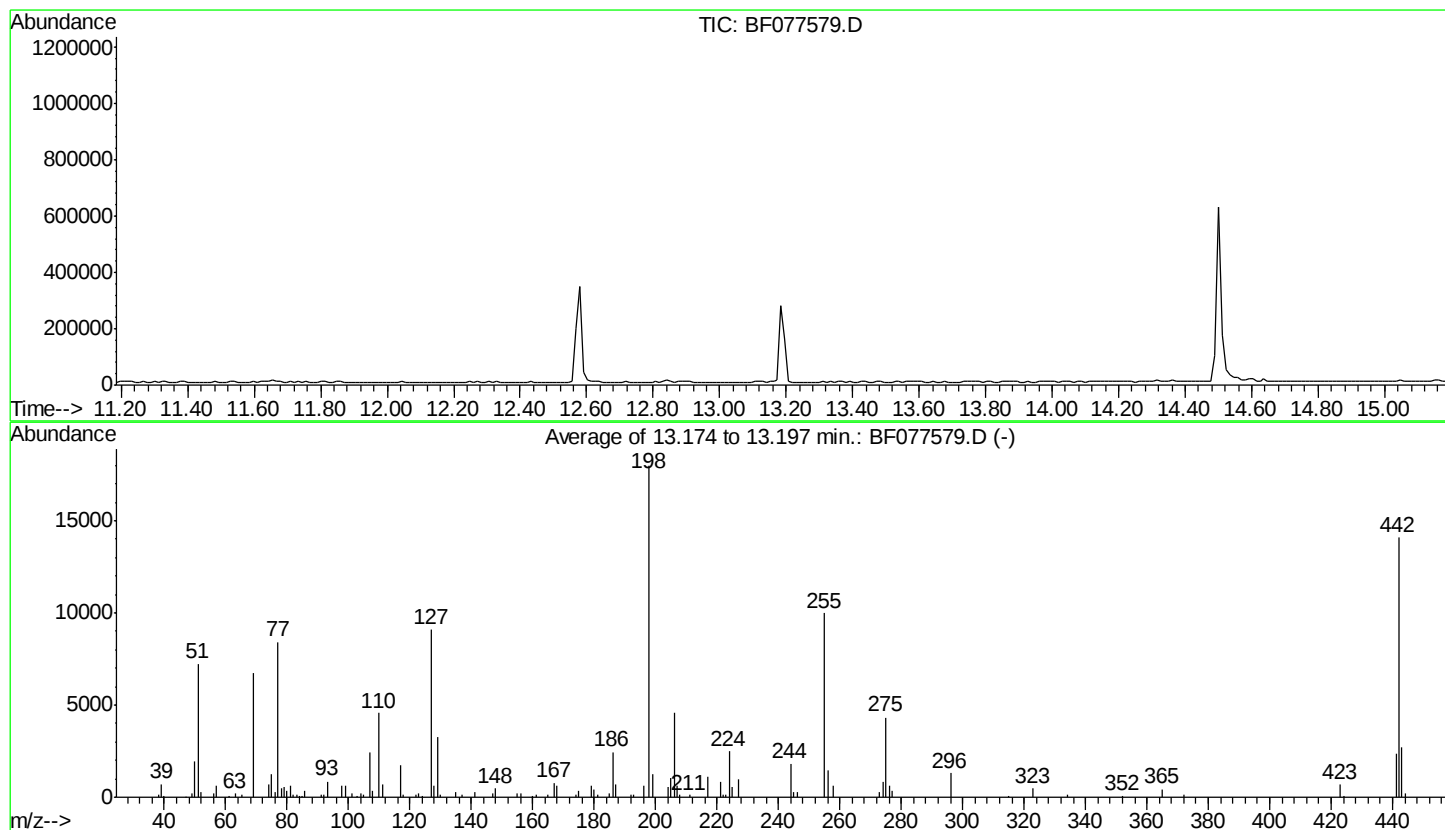

AutoFind: Scans 1075, 1076, 1077; Background Corrected with Scan 1072

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	7238	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.3	6710	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	9072	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17986	PASS
199	198	5	9	7.0	1263	PASS
275	198	10	60	23.9	4305	PASS
365	198	1	100	2.5	448	PASS
441	442	0.01	24	16.8	2371	PASS
442	198	50	100	78.3	14079	PASS
443	442	15	24	19.2	2699	PASS