


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030415\
 Data File : BF077596.D
 Acq On : 4 Mar 2015 23:15
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 04 21:51:23 2015

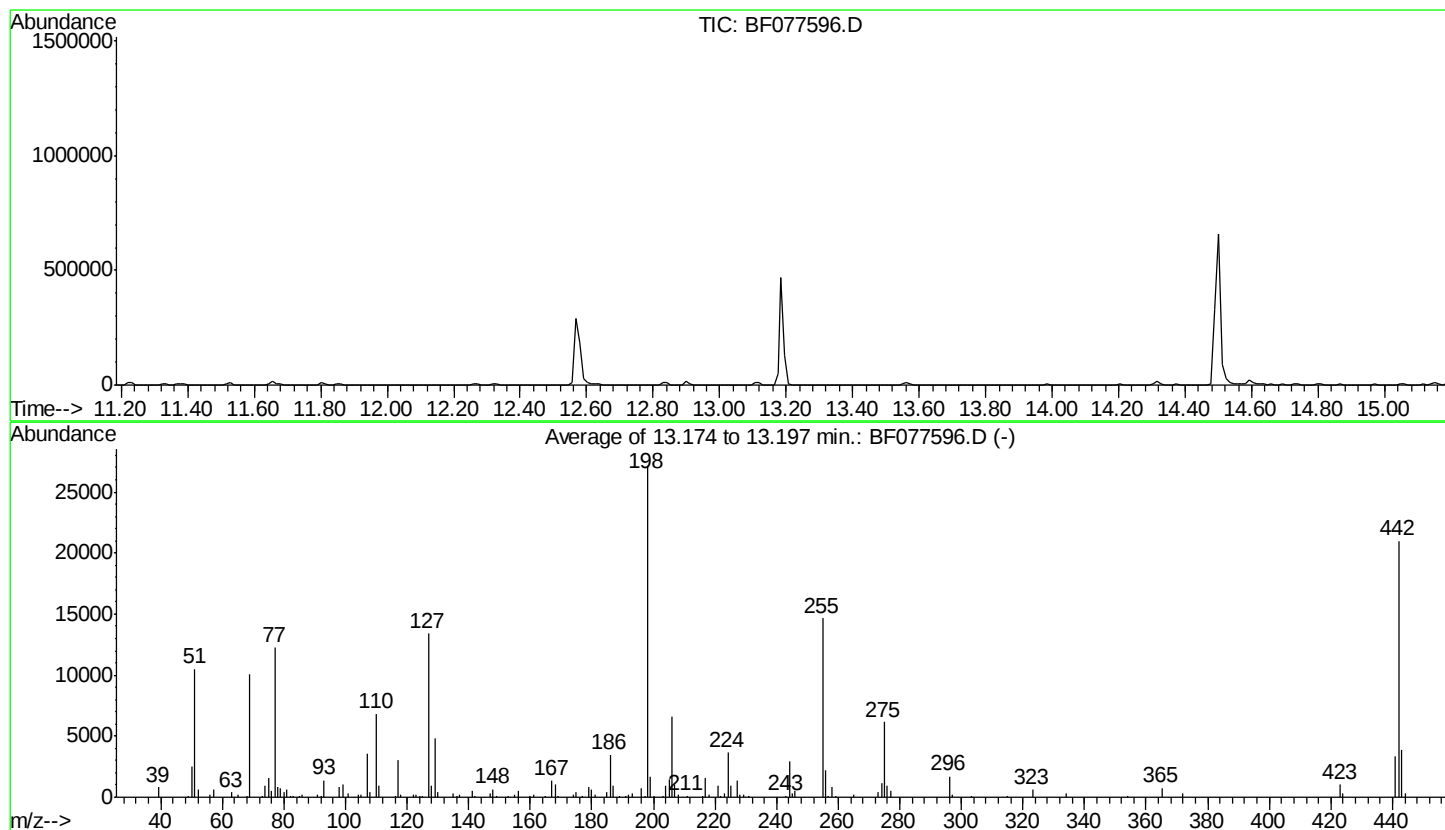

AutoFind: Scans 1075, 1076, 1077; Background Corrected with Scan 1072

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	10491	PASS
68	69	0.00	2	1.3	128	PASS
69	198	0.00	100	37.0	10046	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.3	13382	PASS
197	198	0.00	2	0.5	136	PASS
198	198	100	100	100.0	27154	PASS
199	198	5	9	6.2	1692	PASS
275	198	10	60	22.6	6140	PASS
365	198	1	100	2.8	748	PASS
441	442	0.01	24	16.0	3357	PASS
442	198	50	100	77.4	21013	PASS
443	442	15	24	18.4	3873	PASS