


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030416\
 Data File : BF085201.D
 Acq On : 4 Mar 2016 13:58
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 04 00:54:58 2016

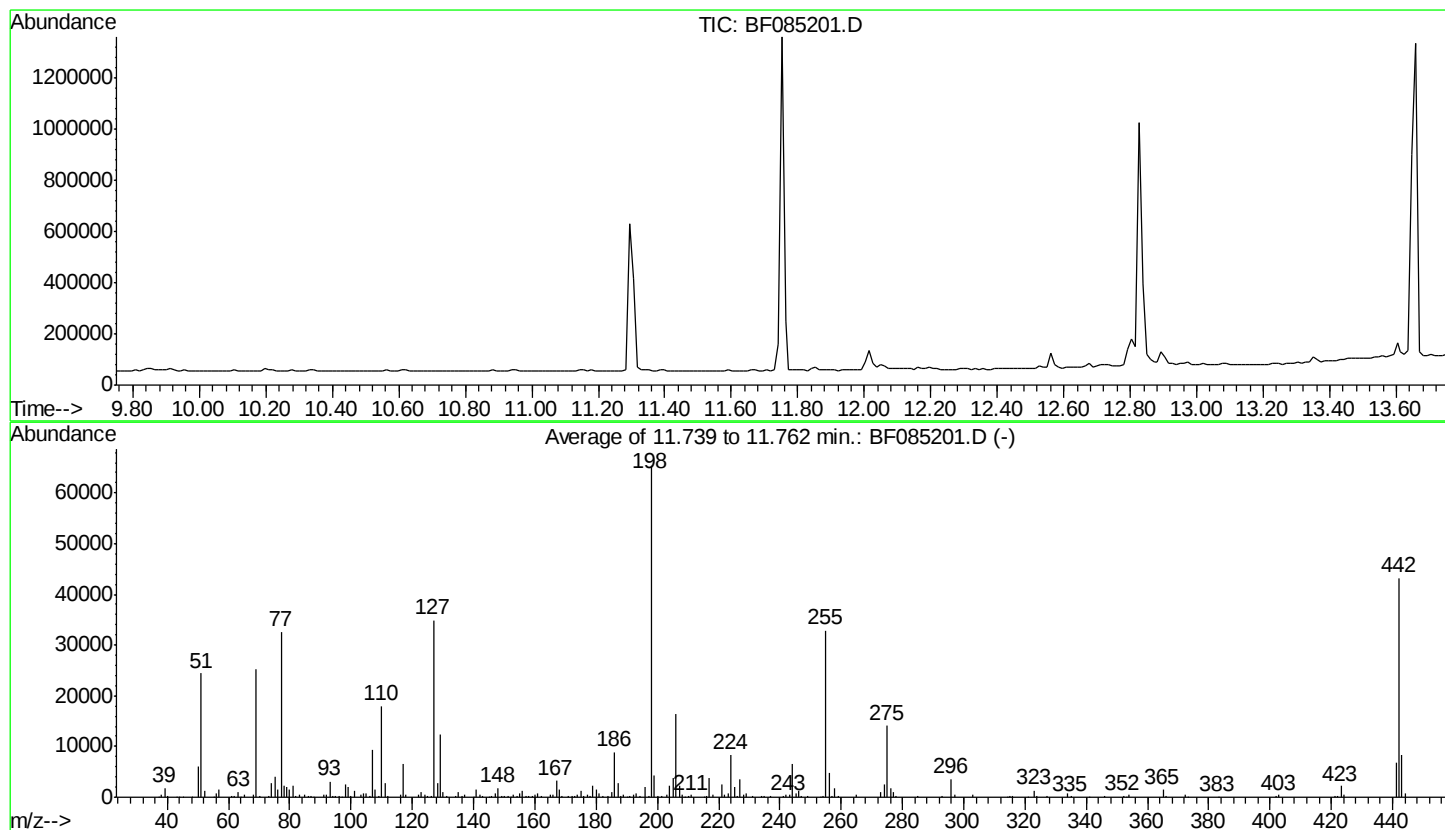

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	24402	PASS
68	69	0.00	2	1.8	451	PASS
69	198	0.00	100	38.6	25208	PASS
70	69	0.00	2	0.7	177	PASS
127	198	10	80	53.3	34855	PASS
197	198	0.00	2	0.5	337	PASS
198	198	100	100	100.0	65378	PASS
199	198	5	9	6.7	4393	PASS
275	198	10	60	21.5	14056	PASS
365	198	1	100	2.3	1474	PASS
441	442	0.01	24	15.6	6738	PASS
442	198	50	100	66.0	43156	PASS
443	442	15	24	19.3	8337	PASS