
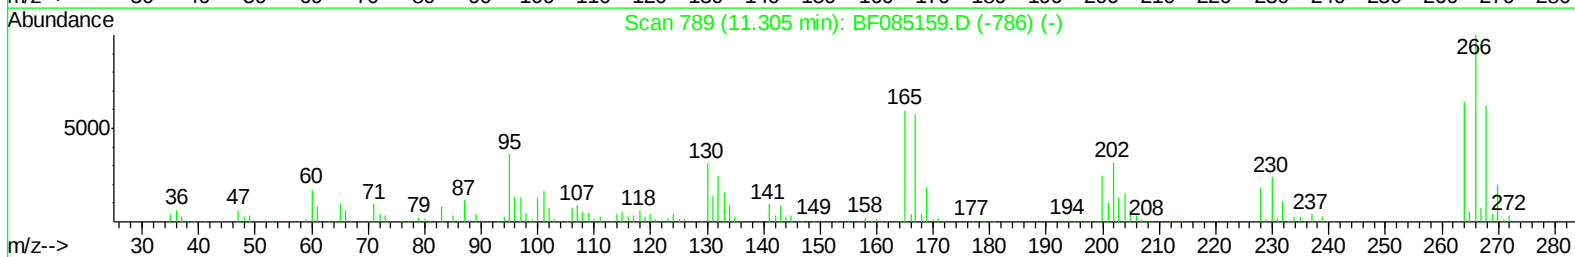
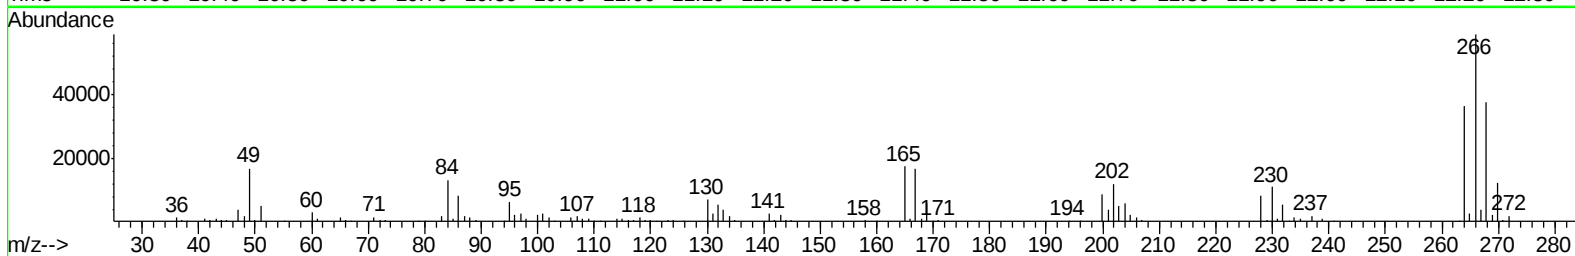


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030416\
Data File : BF085201.D
Acq On : 4 Mar 2016 13:58
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 00:22:54 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

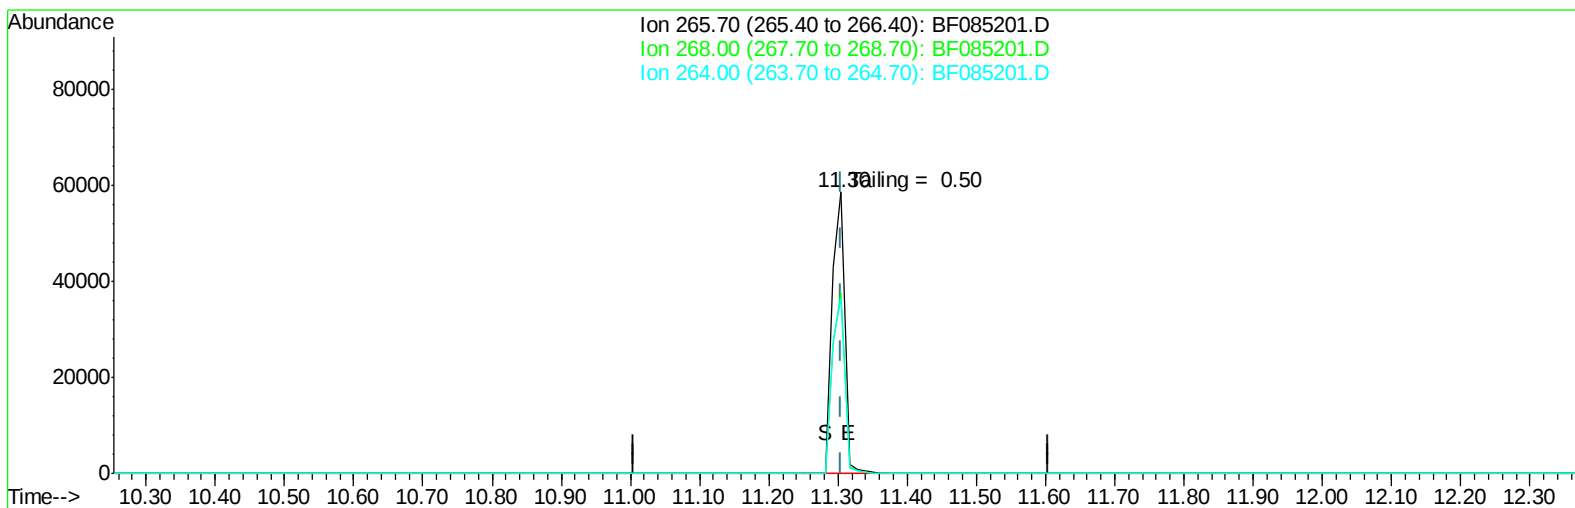

TIC: BF085201.D

(69) Pentachlorophenol (C)




11.305min (+0.000) 39471.48ng

response 72172

Ion	Exp%	Act%
265.70	100	100
268.00	62.50	64.18
264.00	64.30	62.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF030416\
Data File : BF085201.D
Acq On : 4 Mar 2016 13:58
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 00:22:54 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 04 00:54:58 2016
Response via : Initial Calibration

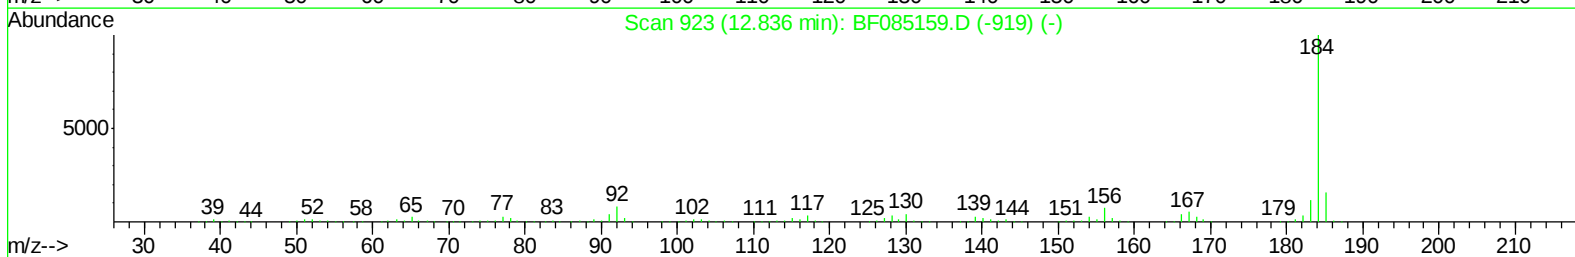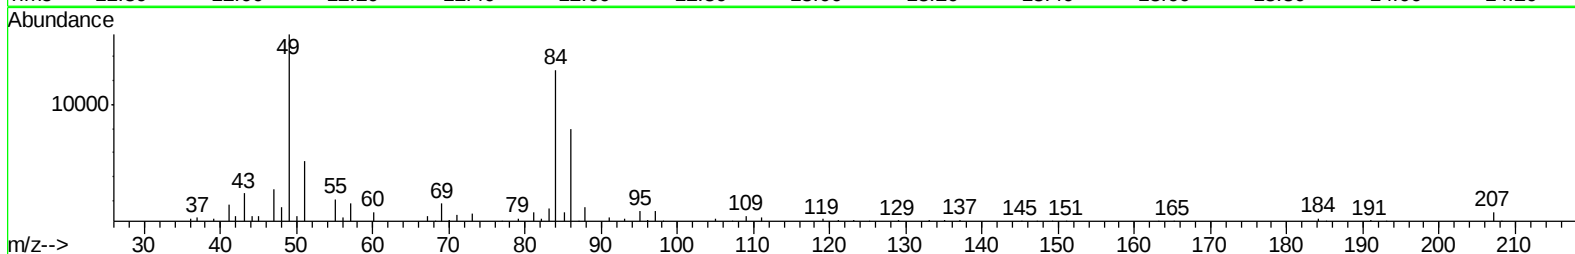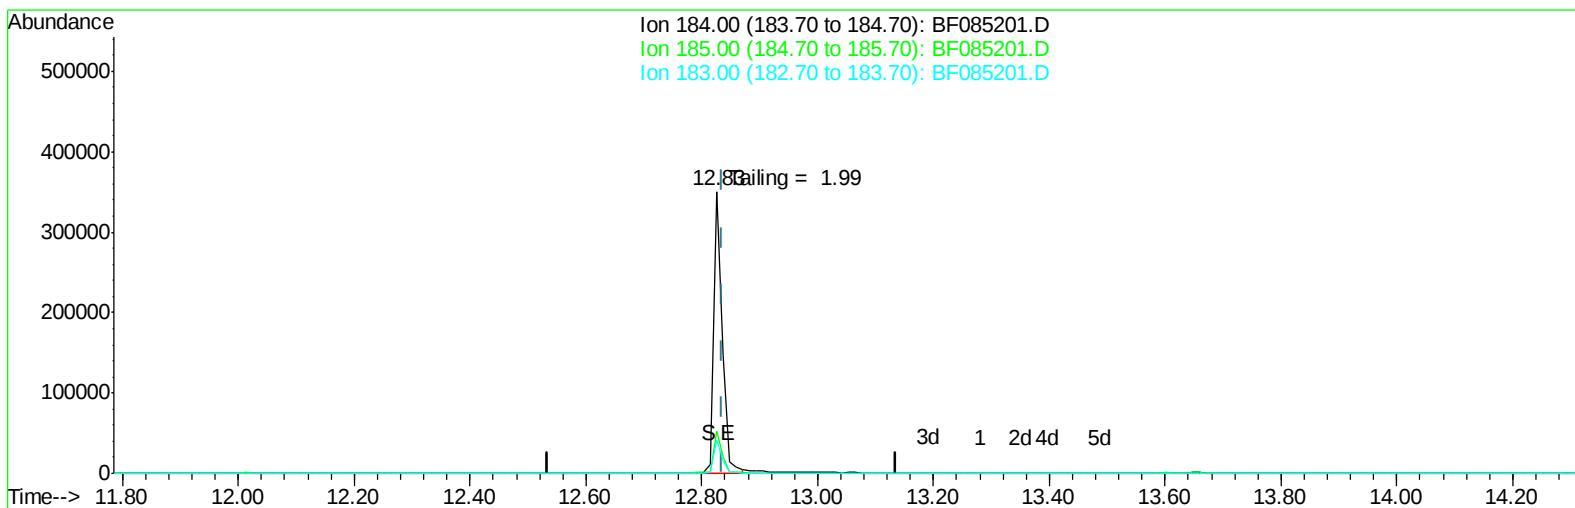

TIC: BF085201.D

(76) Benzidine

13.282min (+0.446) 36.49ng

response 265

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	57.47#
183.00	11.80	0.00#
0.00	0.00	0.00