


Data Path : Z:\HPCHEM1\BNA_F\Data\BF030416\
 Data File : BF085226.D
 Acq On : 5 Mar 2016 2:11
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF030316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 04 00:54:58 2016

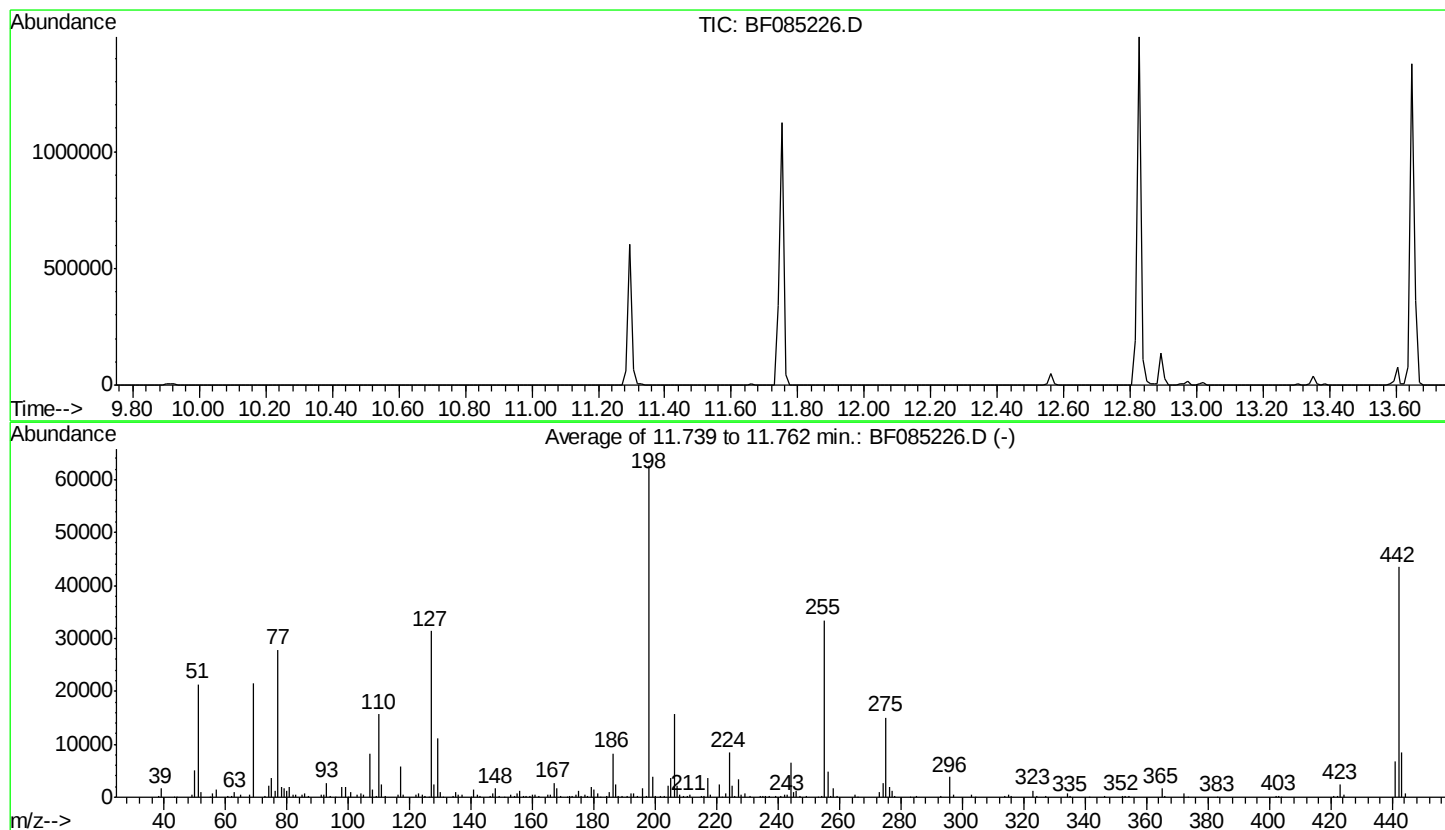

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	21306	PASS
68	69	0.00	2	1.8	393	PASS
69	198	0.00	100	34.5	21621	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	31335	PASS
197	198	0.00	2	0.5	322	PASS
198	198	100	100	100.0	62621	PASS
199	198	5	9	6.3	3951	PASS
275	198	10	60	24.0	15022	PASS
365	198	1	100	2.6	1607	PASS
441	442	0.01	24	15.6	6757	PASS
442	198	50	100	69.3	43406	PASS
443	442	15	24	19.4	8423	PASS