
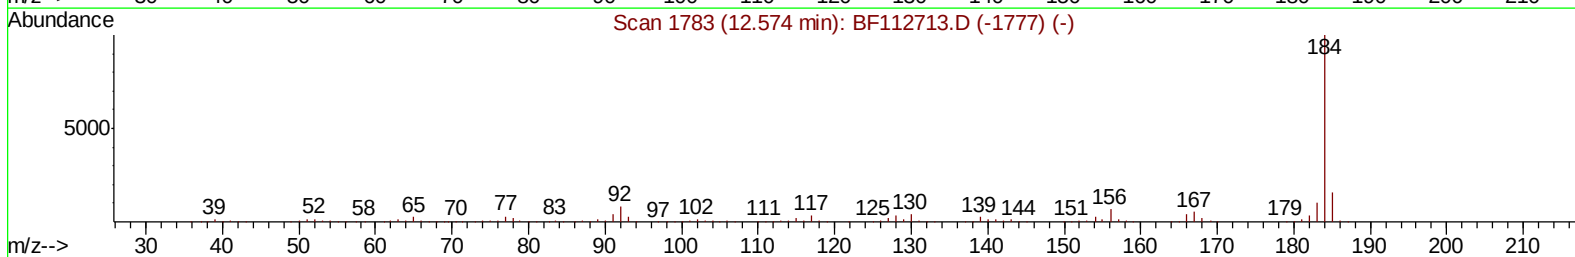
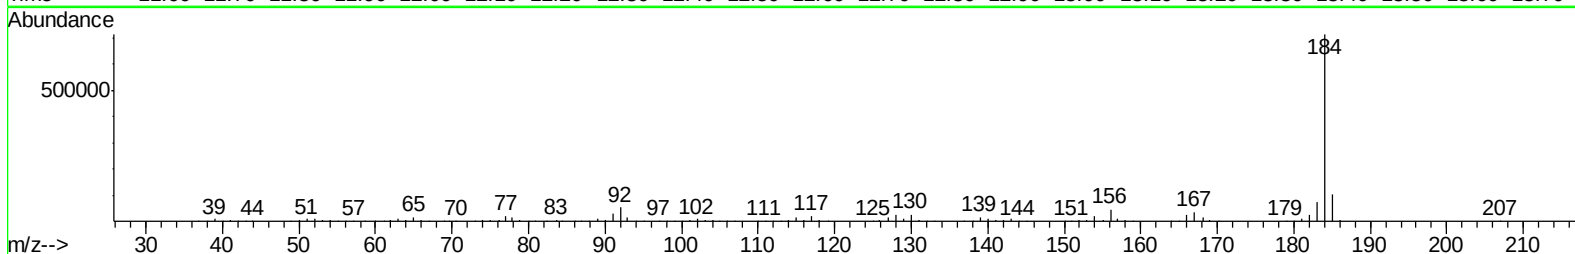


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030419\
Data File : BF112815.D
Acq On : 4 Mar 2019 11:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:14:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 15:40:43 2019
Response via : Initial Calibration

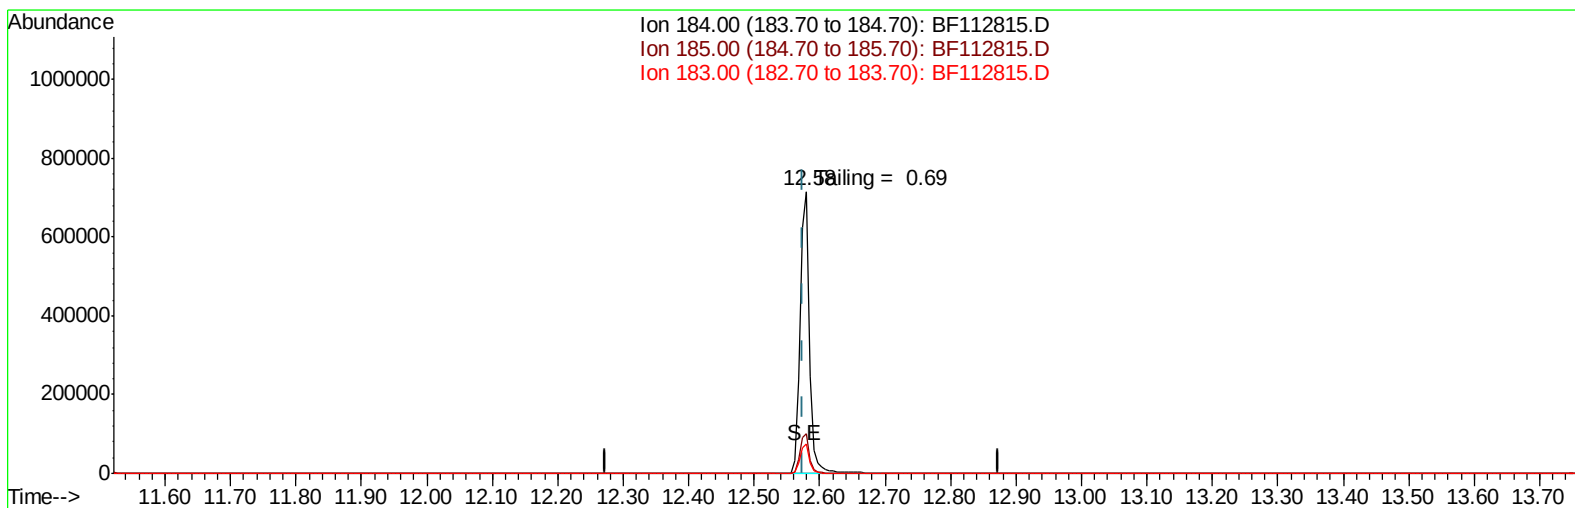

TIC: BF112815.D

(77) Benzidine




12.580min (+0.006) 14273.77ng

response 712407

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.22
183.00	10.70	10.65
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030419\
Data File : BF112815.D
Acq On : 4 Mar 2019 11:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:14:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 15:40:43 2019
Response via : Initial Calibration

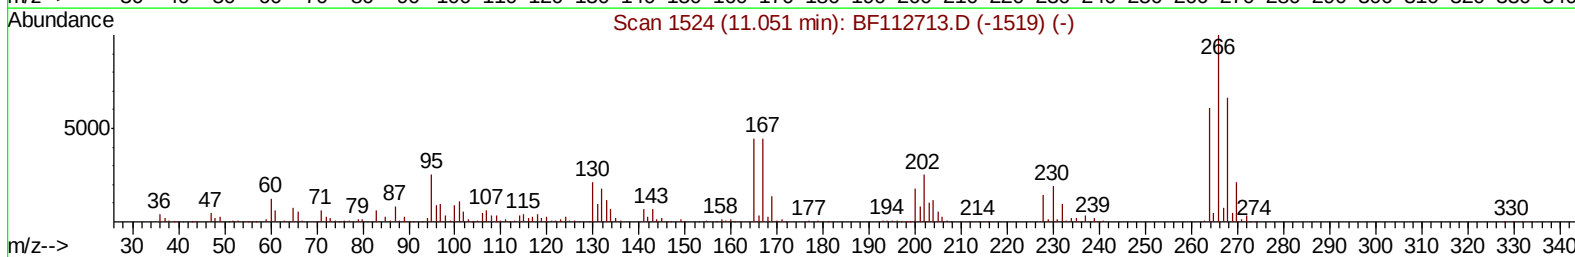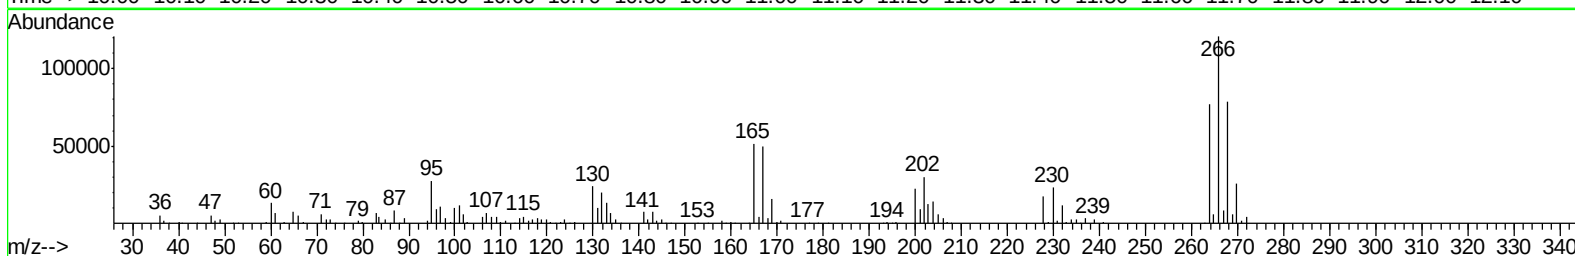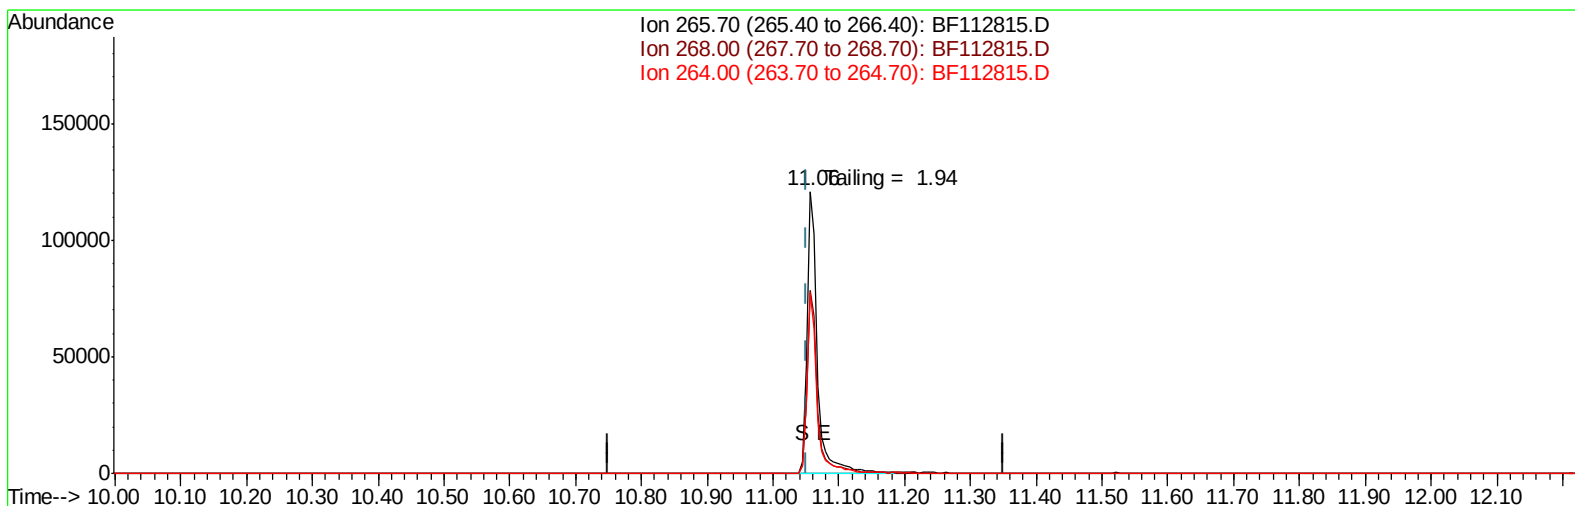

TIC: BF112815.D

(70) Pentachlorophenol (C)

11.057min (+0.006) 0.00ng

response 132419

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.16
264.00	61.10	64.13
0.00	0.00	0.00