
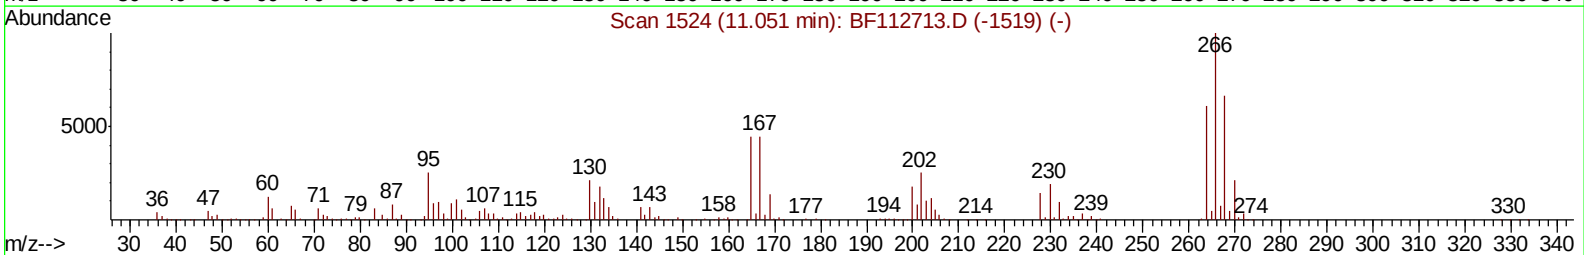
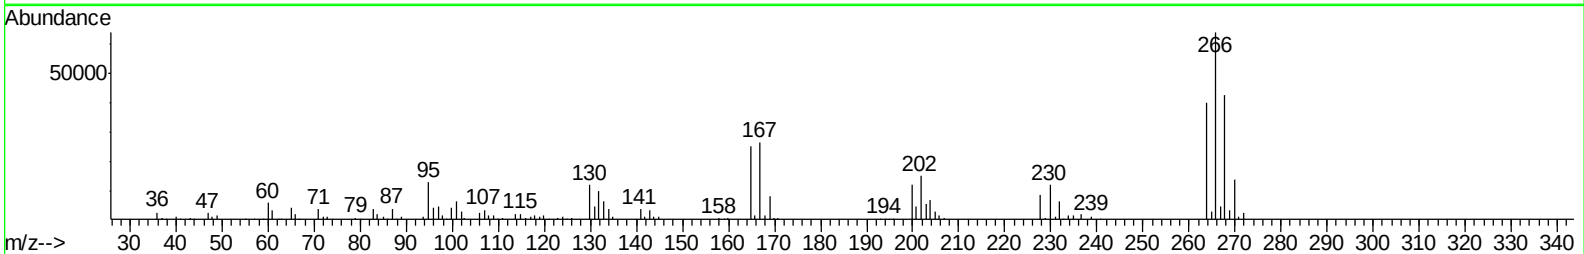


```
Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030419\  
Data File : BF112840.D  
Acq On    : 5 Mar 2019    1:11  
Operator  : JU/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 05 07:12:22 2019
Quant Method : Z:\SV0ASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 15:40:43 2019
Response via : Initial Calibration

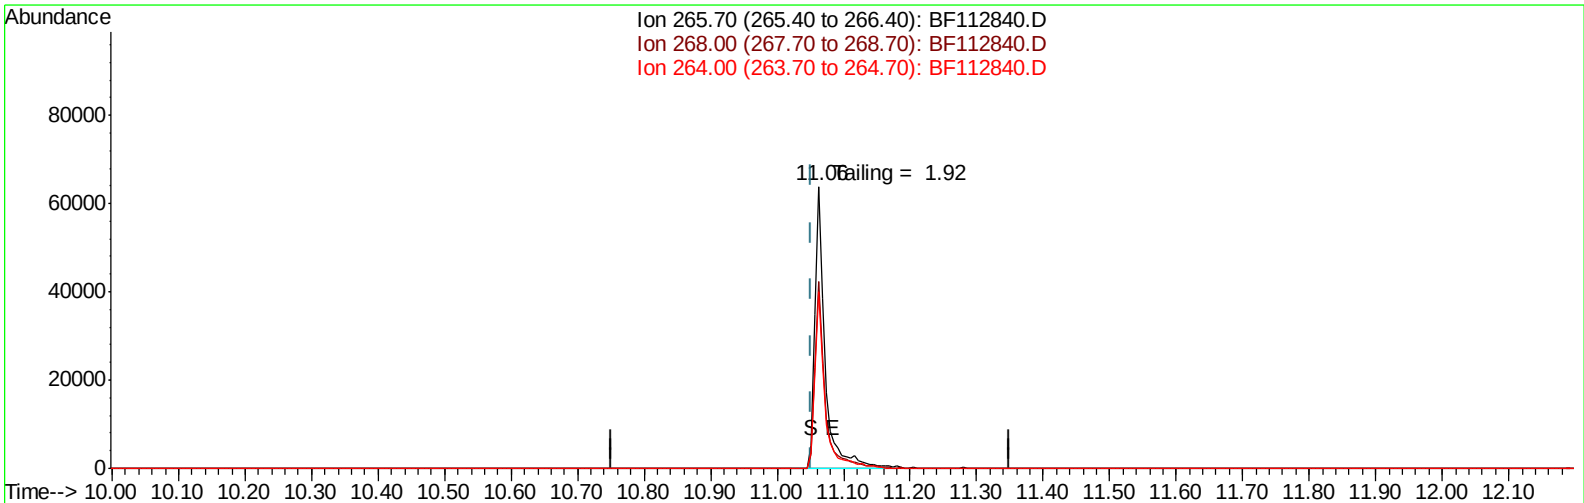

TIC: BF112840.D

(70) Pentachlorophenol (C)




11.063min (+0.012) 0.00ng

response 70364

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.57
264.00	61.10	62.52
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF030419\
Data File : BF112840.D
Acq On : 5 Mar 2019 1:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 07:12:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 15:40:43 2019
Response via : Initial Calibration

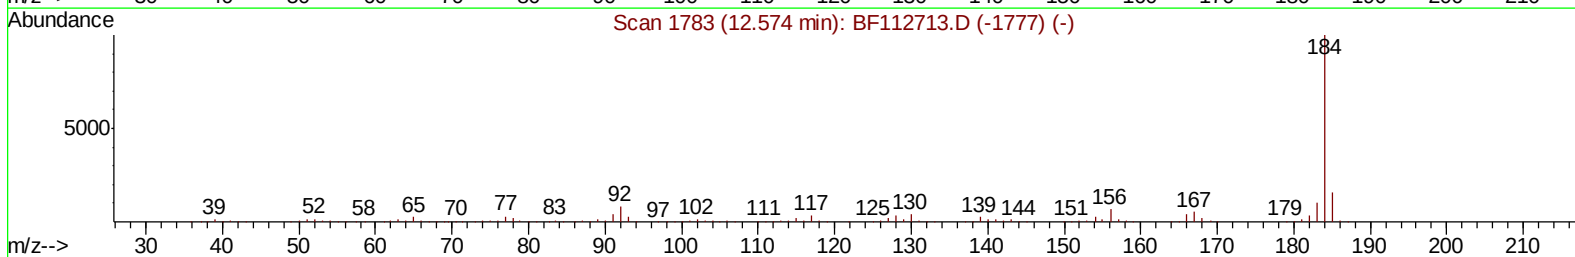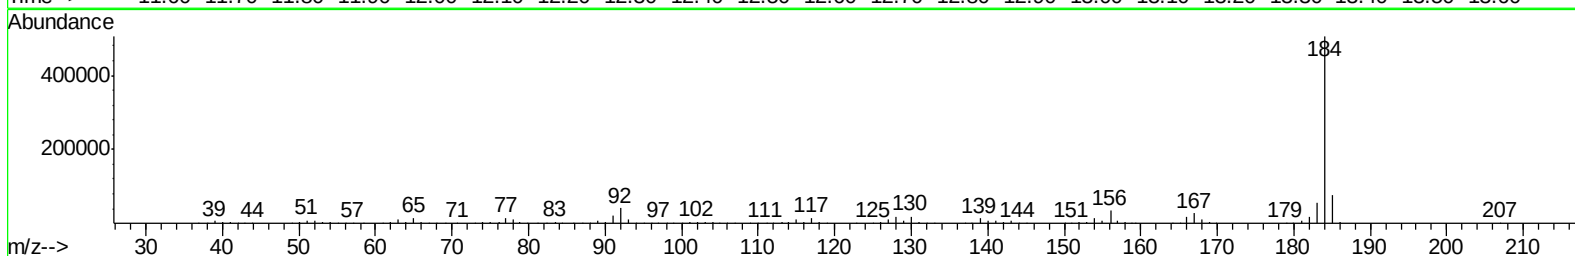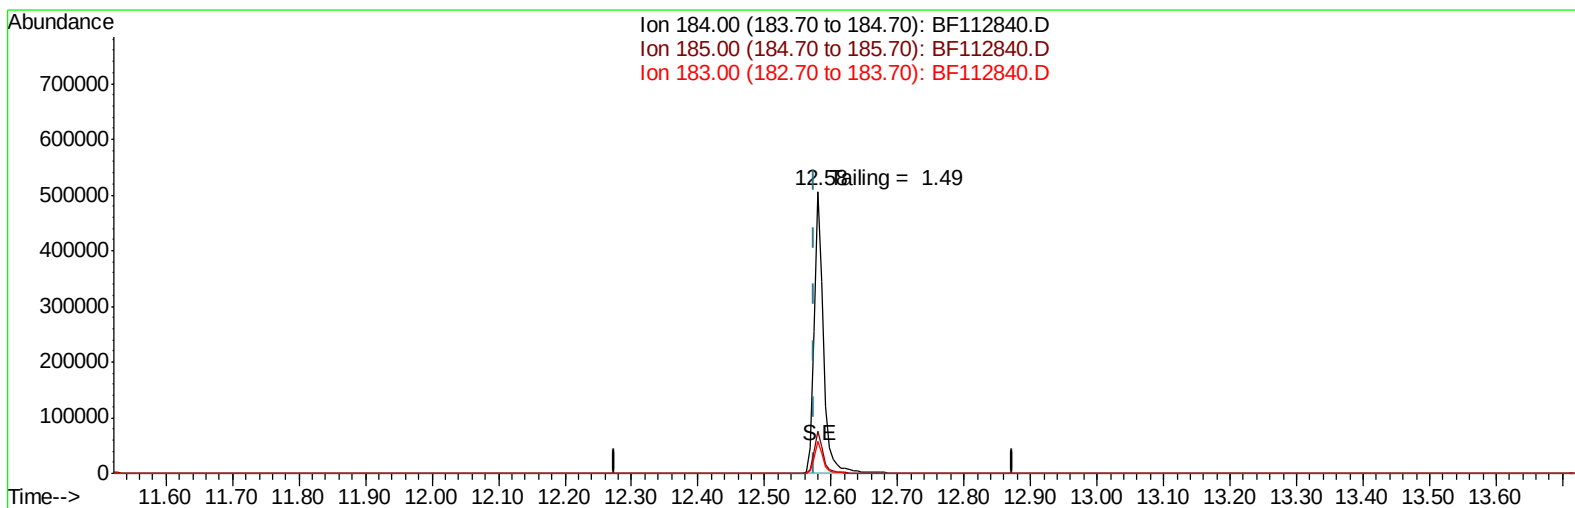

TIC: BF112840.D

(77) Benzidine

12.580min (+0.006) 11142.07ng

response 498296

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.82
183.00	10.70	11.24
0.00	0.00	0.00