


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030419\
 Data File : BF112815.D
 Acq On : 4 Mar 2019 11:04
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 01 15:40:43 2019

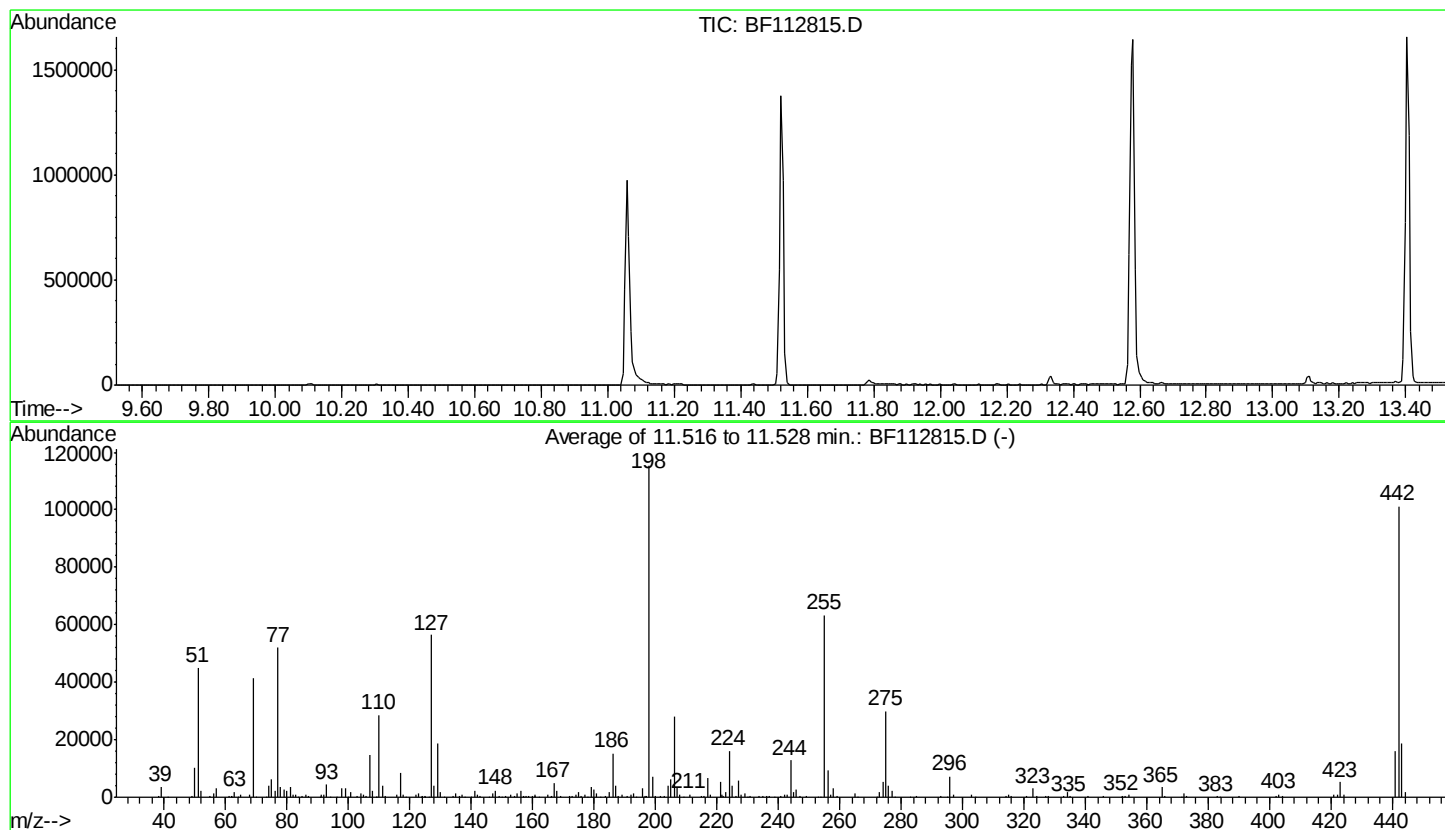

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	45061	PASS
68	69	0.00	2	1.9	784	PASS
69	198	0.00	100	36.0	41490	PASS
70	69	0.00	2	0.4	156	PASS
127	198	10	80	49.0	56490	PASS
197	198	0.00	2	0.3	387	PASS
198	198	100	100	100.0	115352	PASS
199	198	5	9	6.1	7058	PASS
275	198	10	60	26.1	30051	PASS
365	198	1	100	3.0	3497	PASS
441	198	0.01	100	14.0	16205	PASS
442	198	50	100	87.7	101112	PASS
443	442	15	24	18.4	18631	PASS