
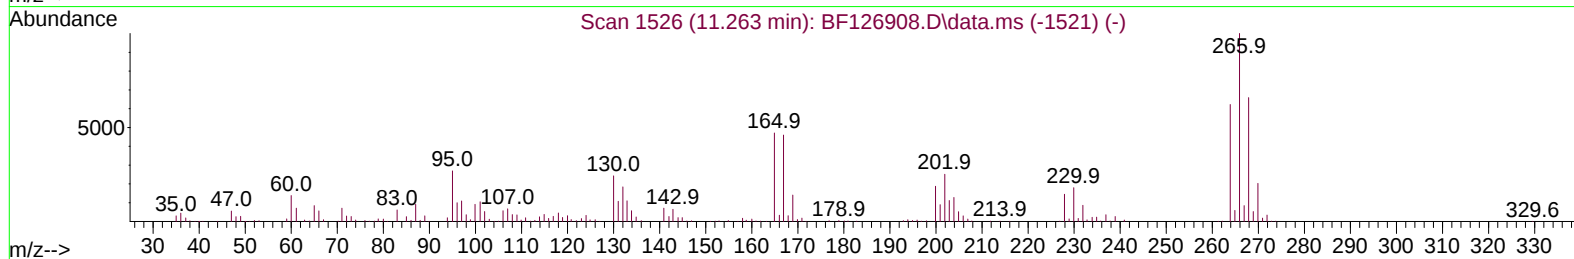
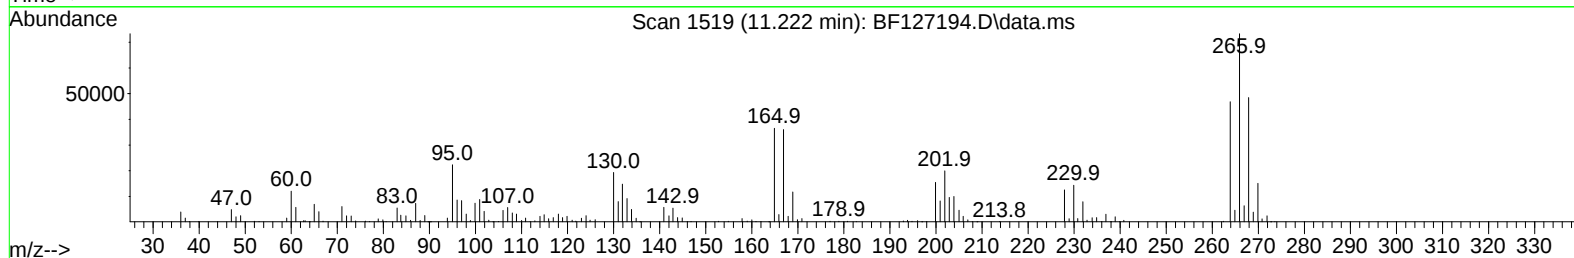


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030422\
Data File : BF127194.D
Acq On : 04 Mar 2022 09:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 05:12:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 02:16:58 2022
Response via : Initial Calibration

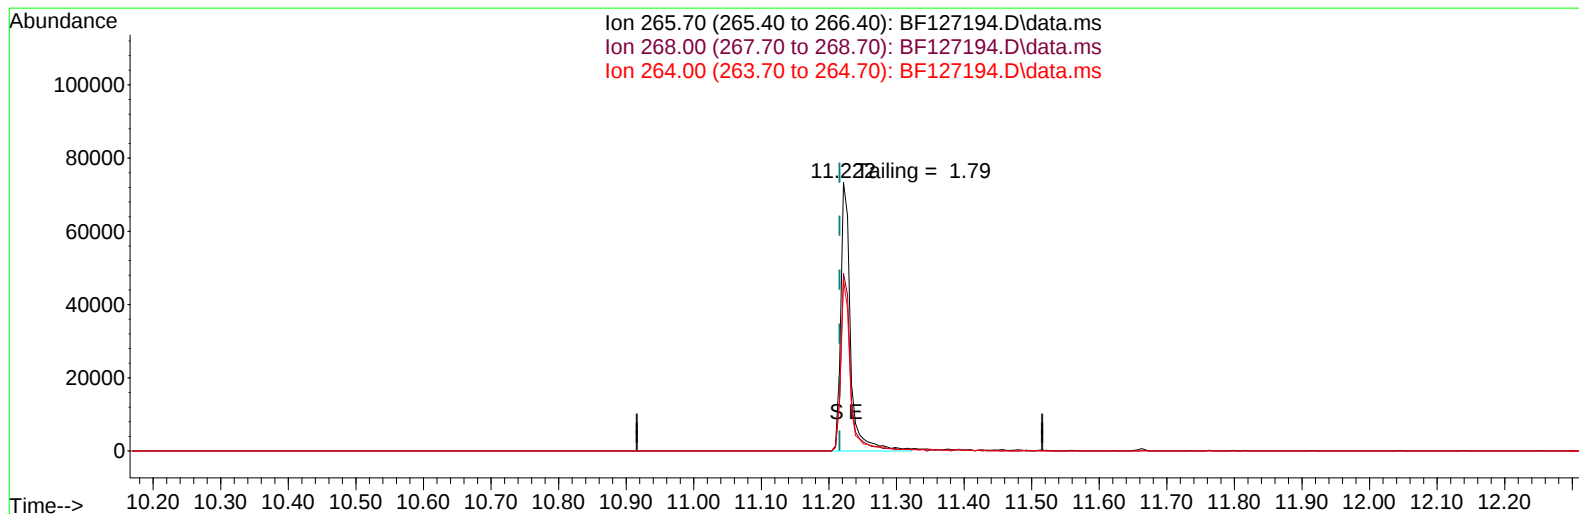

TIC: BF127194.D\data.ms

(70) Pentachlorophenol (C)




11.222min (+ 0.006) 22030.80 ng

response 73484

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.15
264.00	63.00	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030422\
 Data File : BF127194.D
 Acq On : 04 Mar 2022 09:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 05 05:12:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 02:16:58 2022
 Response via : Initial Calibration

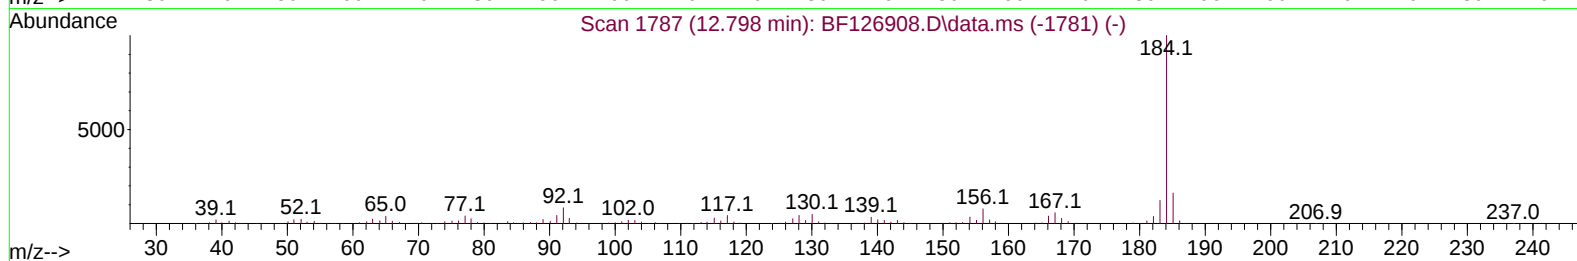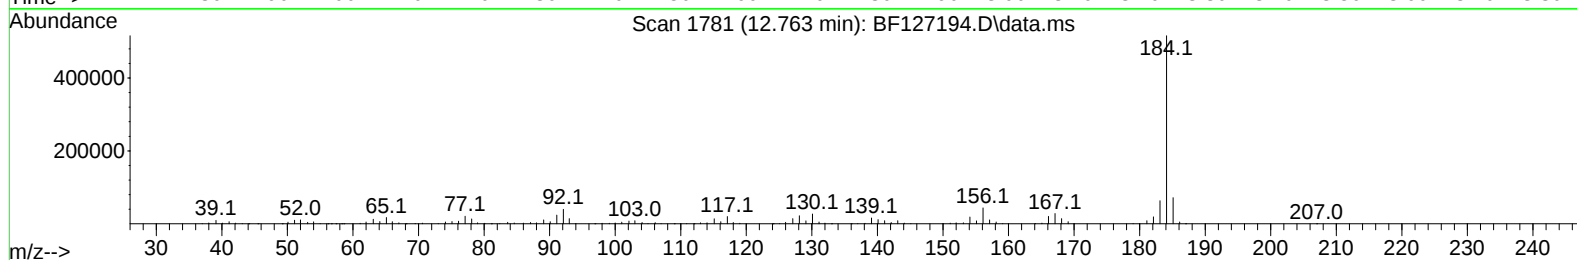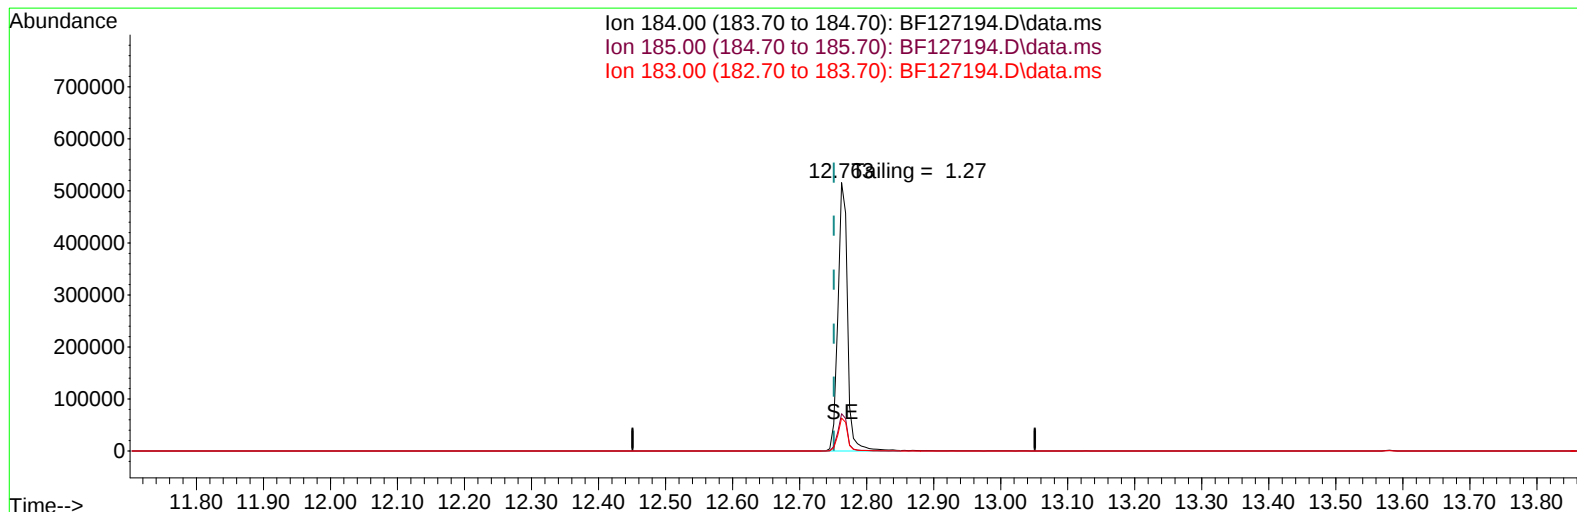

TIC: BF127194.D\data.ms

(77) Benzidine**12.763min (+ 0.012) 262093.04 ng****response 512824**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.93
183.00	10.20	12.27#
0.00	0.00	0.00