


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030422\
 Data File : BF127194.D
 Acq On : 04 Mar 2022 09:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 05 02:16:58 2022

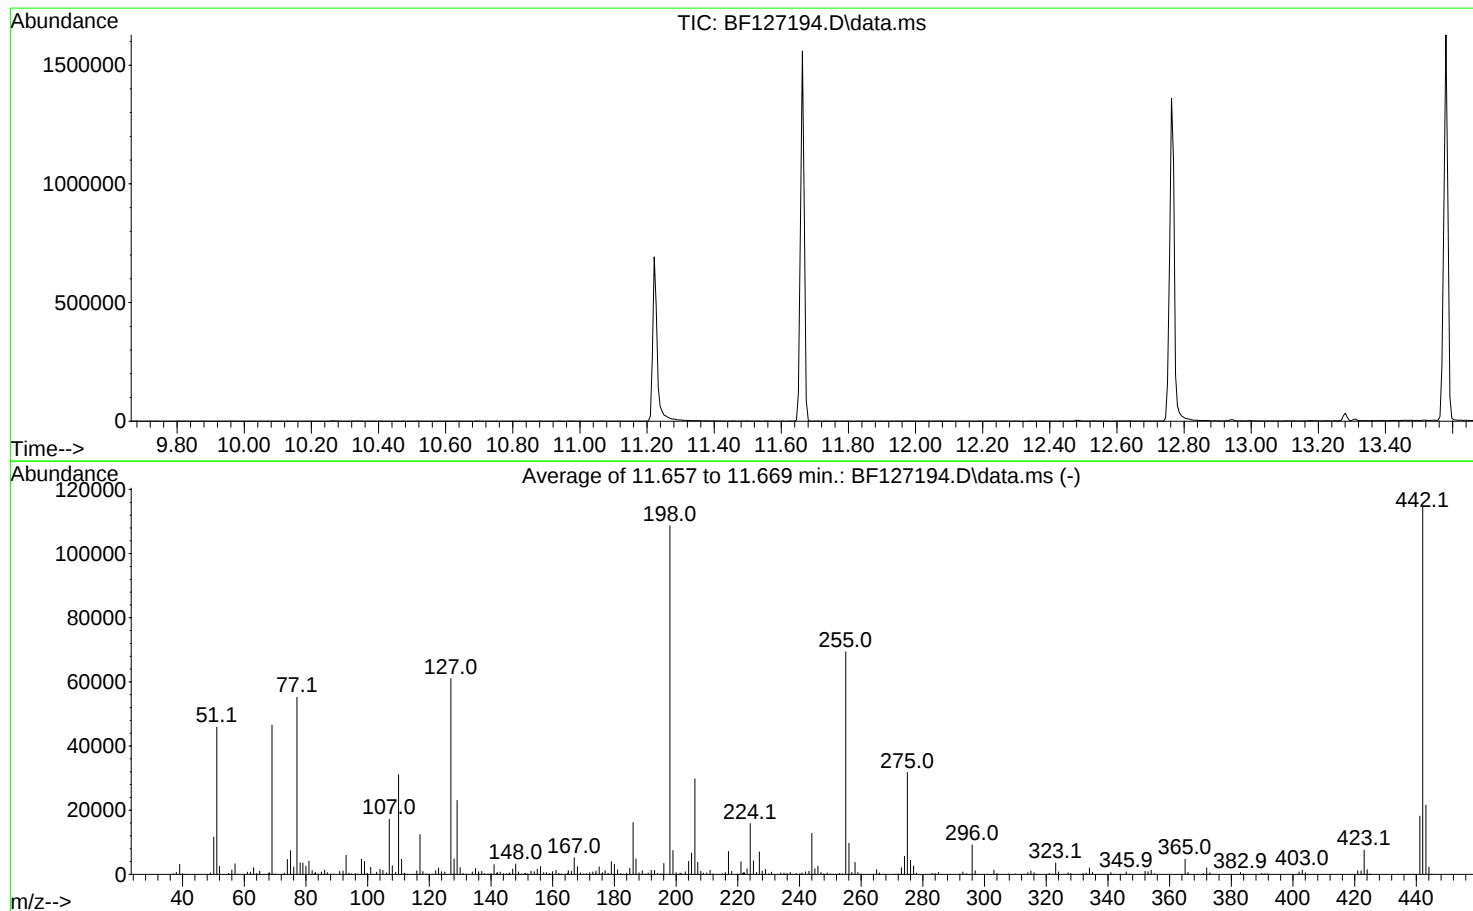

AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	45877	PASS
68	69	0.00	2	1.0	468	PASS
69	198	0.00	100	42.8	46544	PASS
70	69	0.00	2	0.4	176	PASS
127	198	10	80	56.2	61067	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	108707	PASS
199	198	5	9	6.8	7414	PASS
275	198	10	60	29.2	31771	PASS
365	198	1	100	4.3	4704	PASS
441	198	0.01	100	16.7	18180	PASS
442	442	50	100	100.0	114688	PASS
443	442	15	24	18.8	21530	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/4/2022	BNA_F	<u>BF127194.D</u>
Compound Name	Response	Retention Time
DDT	245478	13.58
DDD	6363	13.28
DDE	989	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7352	252830	2.91

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030422\
 Data File : BF127194.D
 Acq On : 04 Mar 2022 09:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 05 05:12:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 05 02:16:58 2022
 Response via : Initial Calibration

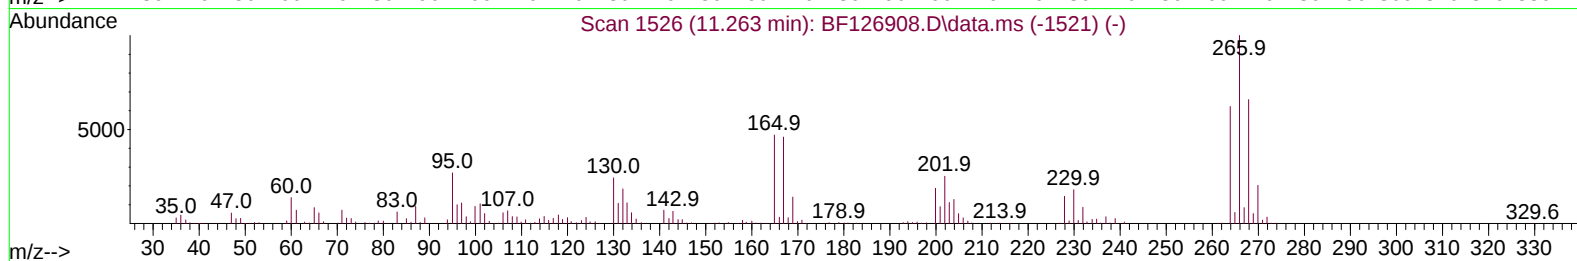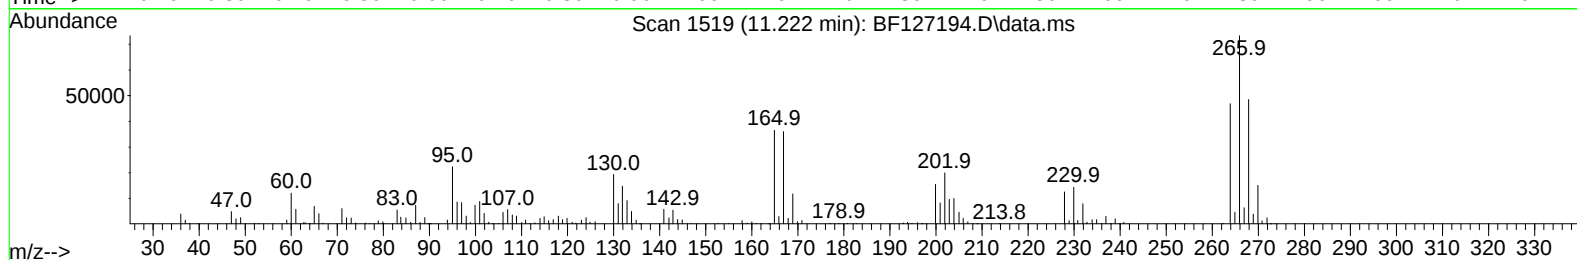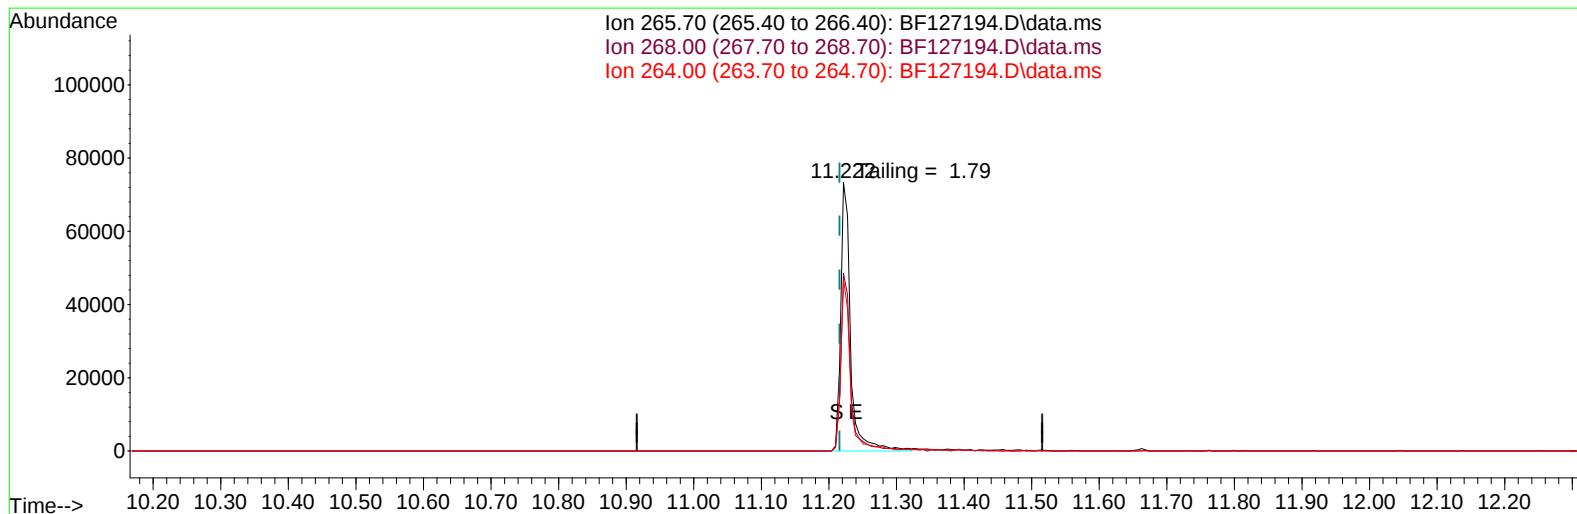

TIC: BF127194.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.006) 22030.80 ng




response 73484

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.15
264.00	63.00	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030422\
Data File : BF127194.D
Acq On : 04 Mar 2022 09:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 05 05:12:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 05 02:16:58 2022
Response via : Initial Calibration

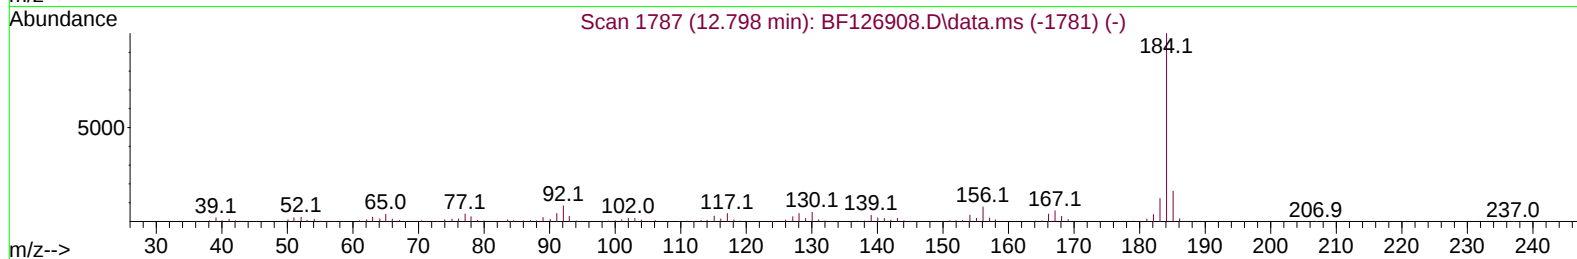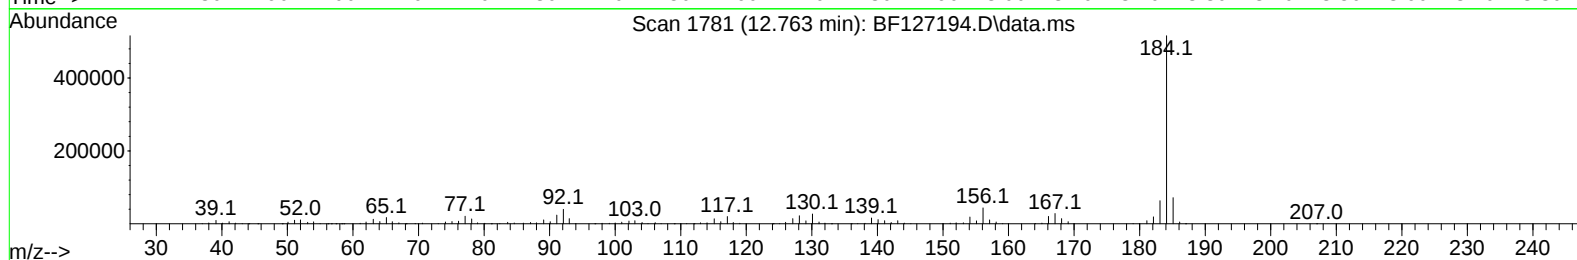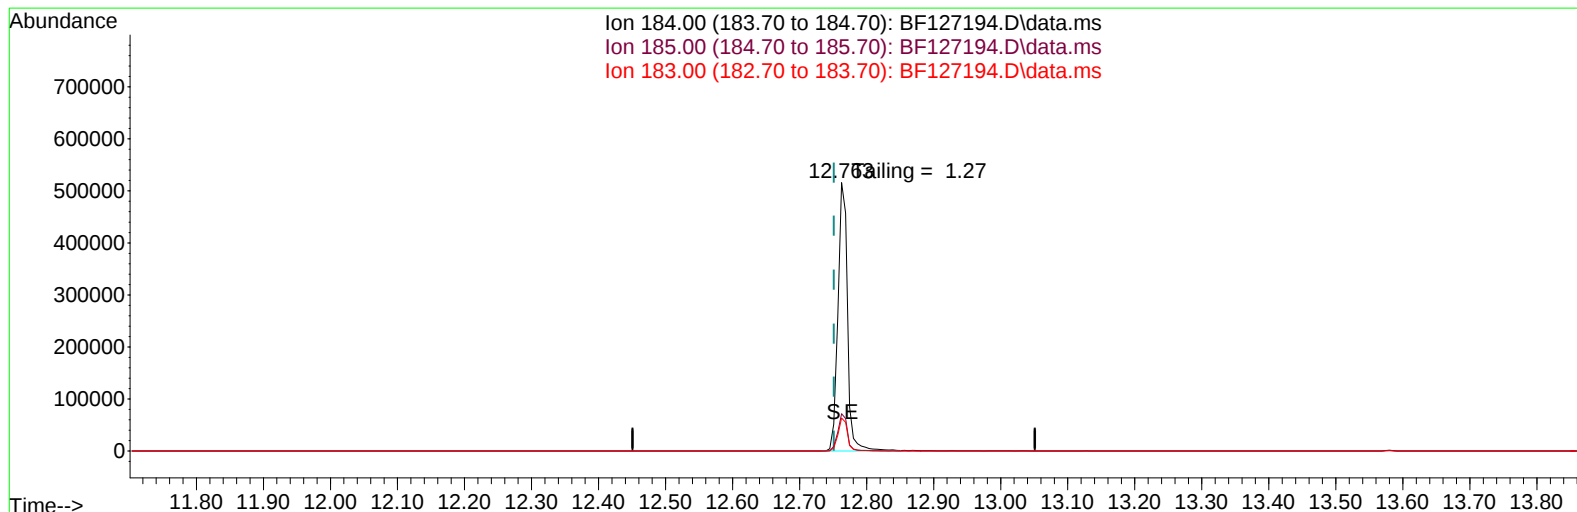

TIC: BF127194.D\data.ms

(77) Benzidine

12.763min (+ 0.012) 262093.04 ng

response 512824

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.93
183.00	10.20	12.27#
0.00	0.00	0.00