

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030424\
 Data File : BF137485.D
 Acq On : 04 Mar 2024 17:19
 Operator : CG\JU
 Sample : P1662-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ETGI-352

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.028	156	160	177	rVB	78048	160375	1.87%	0.292%
2	5.140	515	519	535	rVB	879757	1583837	18.46%	2.885%
3	5.528	580	585	588	rBV	6567634	7096808	82.71%	12.928%
4	6.504	746	751	754	rBV	6187168	6910177	80.53%	12.588%
5	6.857	808	811	830	rBV	1720620	1485693	17.31%	2.707%
6	7.422	901	907	920	rBV	4669804	5236518	61.03%	9.540%
7	7.528	921	925	936	rVB	146452	210261	2.45%	0.383%
8	8.128	1023	1027	1042	rBV	2195763	2006229	23.38%	3.655%
9	9.210	1206	1211	1215	rBV	7806956	8466735	98.67%	15.424%
10	9.886	1322	1326	1330	rBV	2761603	2299832	26.80%	4.190%
11	10.686	1457	1462	1465	rBV	5306413	5126793	59.75%	9.340%
12	11.380	1576	1580	1603	rBV	2583547	2322461	27.07%	4.231%
13	12.739	1808	1811	1822	rBV	327713	443770	5.17%	0.808%
14	12.992	1848	1854	1857	rBV	8080164	8580844	100.00%	15.632%
15	13.157	1879	1882	1890	rBV	67979	106484	1.24%	0.194%
16	13.504	1937	1941	1950	rBV	193876	244402	2.85%	0.445%
17	14.039	2029	2032	2045	rBV	1369520	1363033	15.88%	2.483%
18	15.568	2287	2292	2301	rBV	886140	1248584	14.55%	2.275%




Sum of corrected areas: 54892836

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030424\
Data File : BF137485.D
Acq On : 04 Mar 2024 17:19
Operator : CG\JU
Sample : P1662-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ETGI-352

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

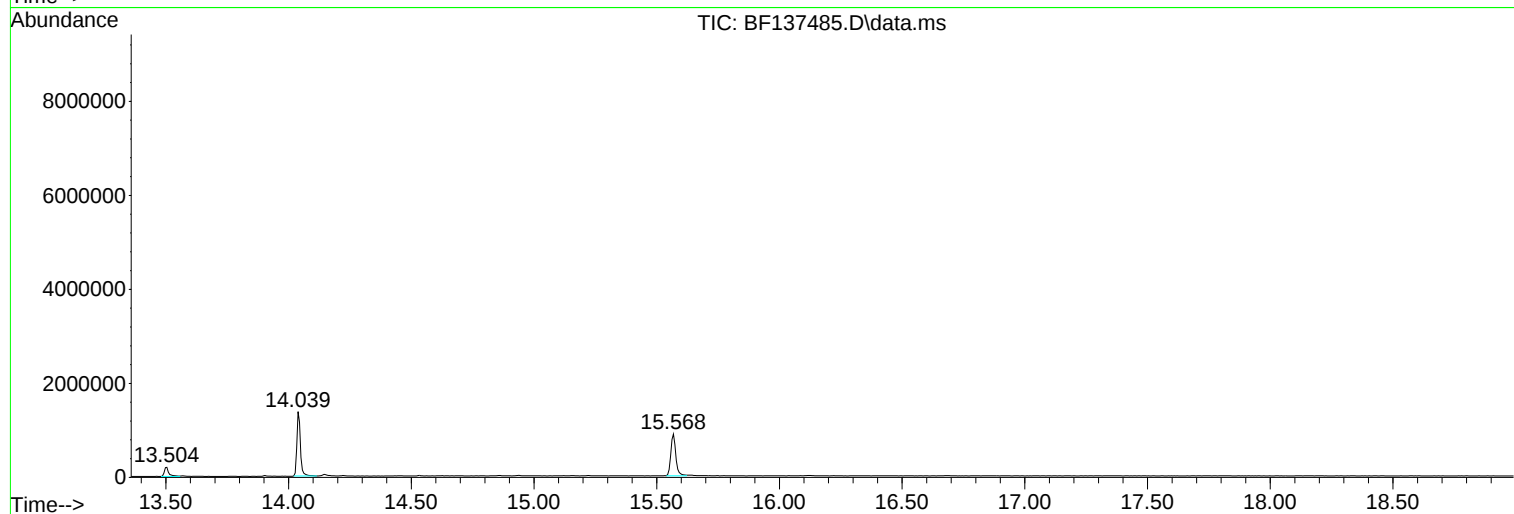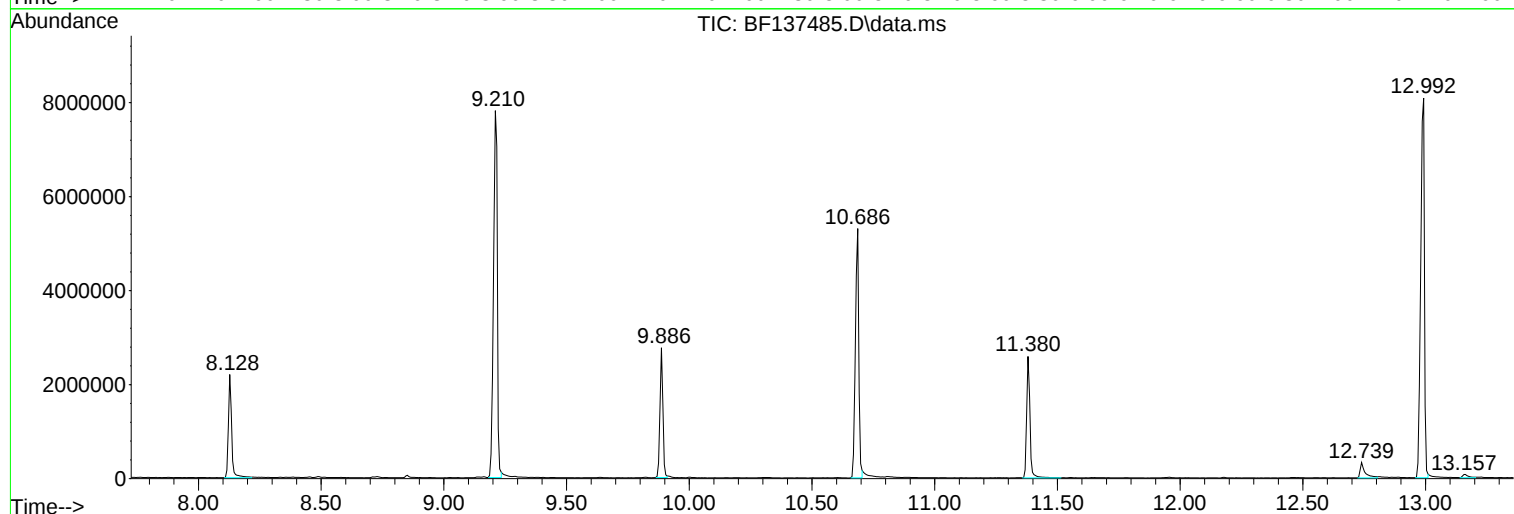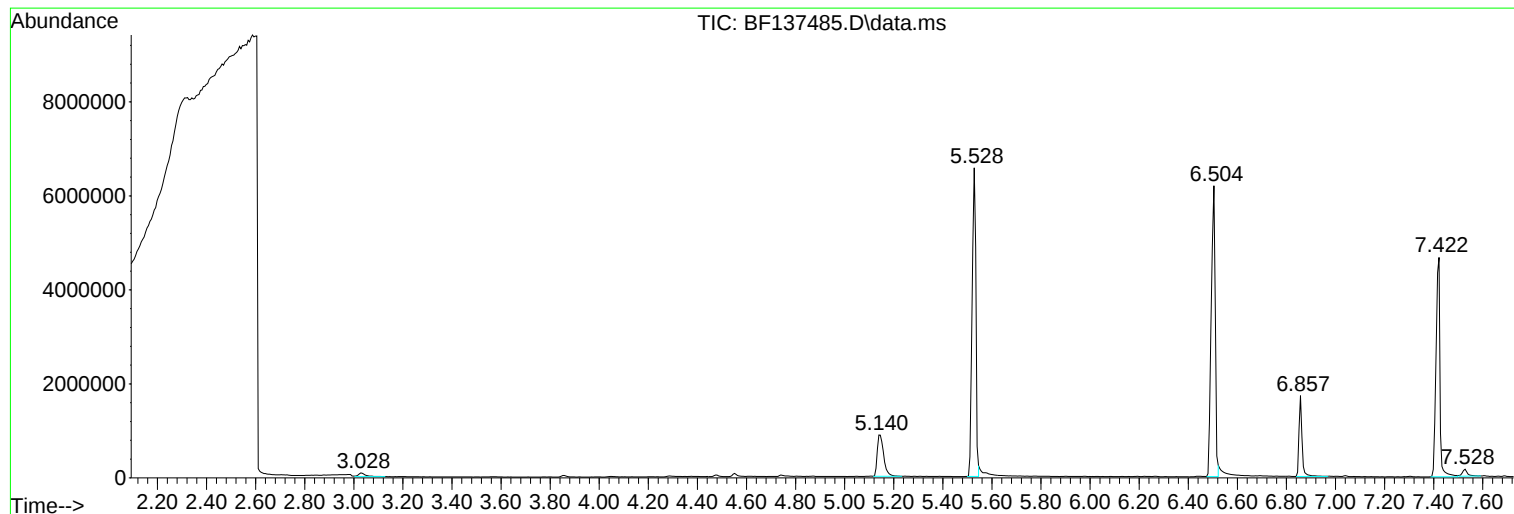

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030424\
Data File : BF137485.D
Acq On : 04 Mar 2024 17:19
Operator : CG\JU
Sample : P1662-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ETGI-352

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030424\
Data File : BF137485.D
Acq On : 04 Mar 2024 17:19
Operator : CG\JU
Sample : P1662-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ETGI-352

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------