
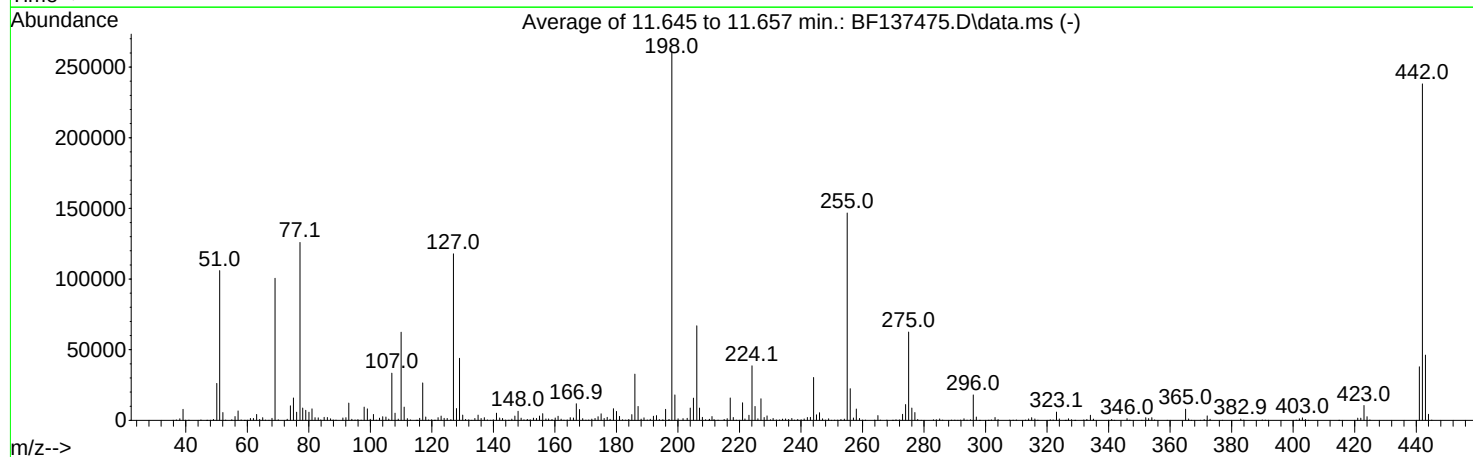


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030424\
Data File : BF137475.D
Acq On : 04 Mar 2024 12:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 04 00:26:53 2024

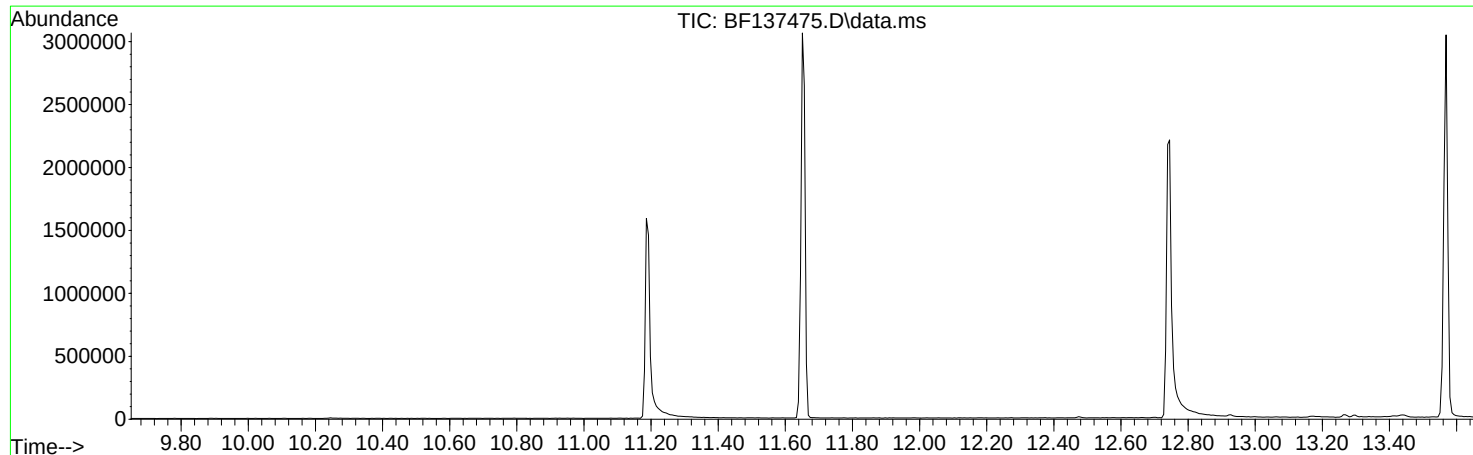




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	105963	PASS
68	69	0.00	2	1.4	1446	PASS
69	198	0.00	100	38.6	100587	PASS
70	69	0.00	2	0.5	491	PASS
127	198	10	80	45.3	117931	PASS
197	198	0.00	2	0.2	547	PASS
198	198	100	100	100.0	260317	PASS
199	198	5	9	6.9	17981	PASS
275	198	10	60	24.0	62571	PASS
365	198	1	100	3.1	7988	PASS
441	198	0.01	100	14.6	37888	PASS
442	442	50	100	100.0	238115	PASS
443	442	15	24	19.4	46208	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030424\
Data File : BF137475.D
Acq On : 04 Mar 2024 12:18
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 04 13:08:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 04 00:26:53 2024
Response via : Initial Calibration

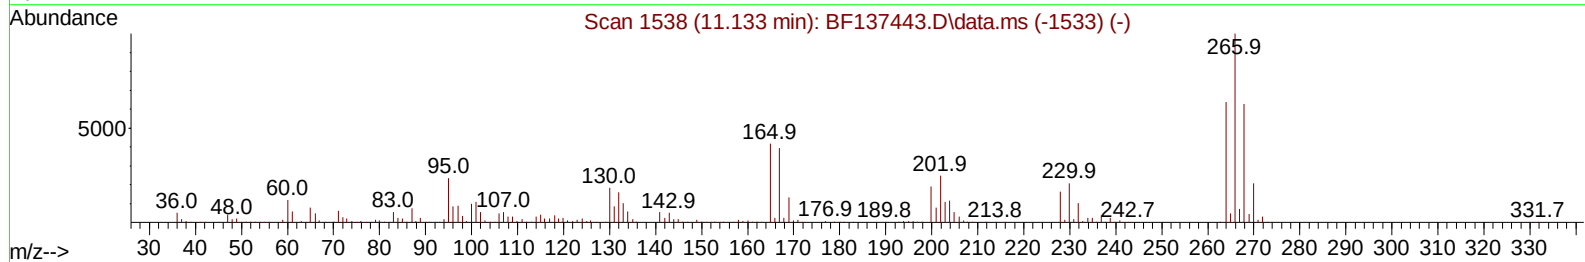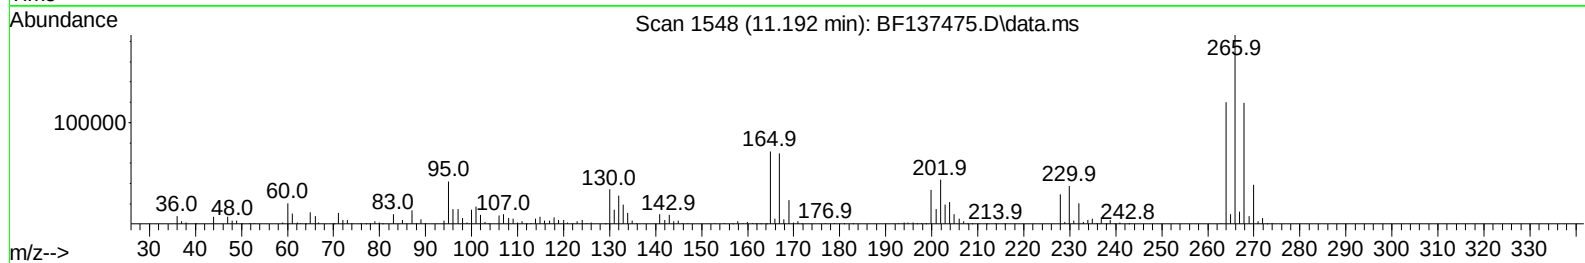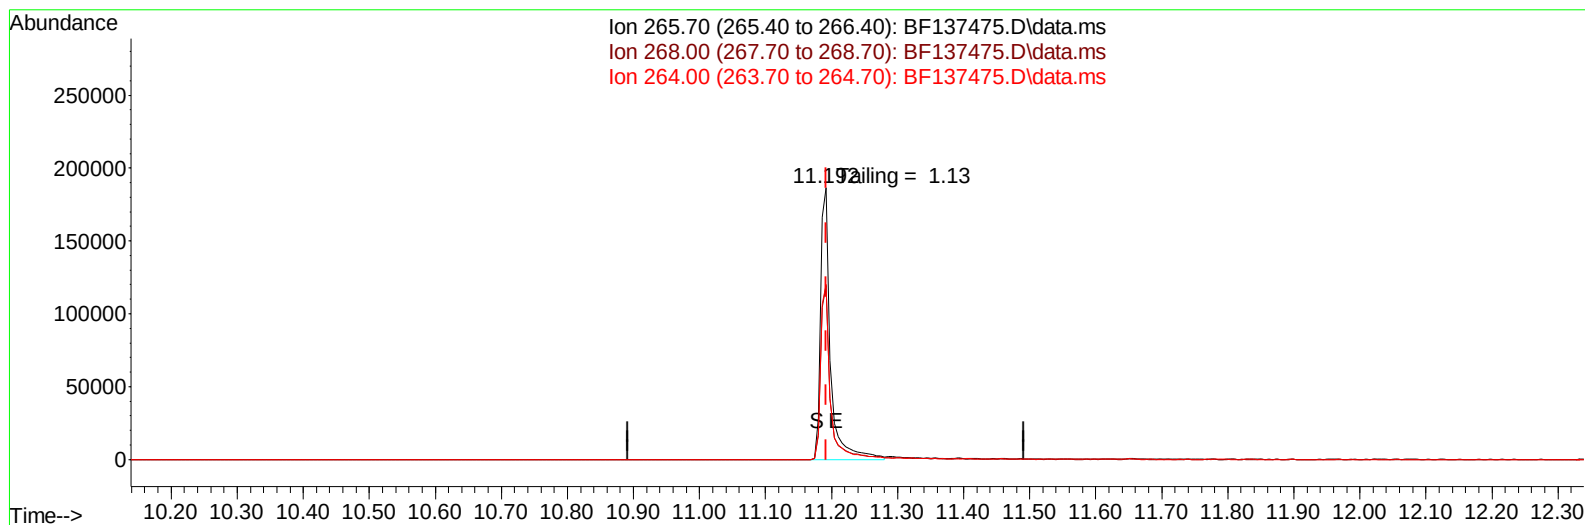

TIC: BF137475.D\data.ms

(70) Pentachlorophenol (C)

11.192min (-0.000) 30948.15 ng

response 199638

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	64.14
264.00	63.60	64.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/4/2024	BNA_F	<u>BF137475.D</u>
Compound Name	Response	Retention Time
DDT	460273	13.568
DDD	6819	13.268
DDE	1921	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8740	469013	1.86

Instrument :
BNA_F
ClientSampleId :
DFTPP