
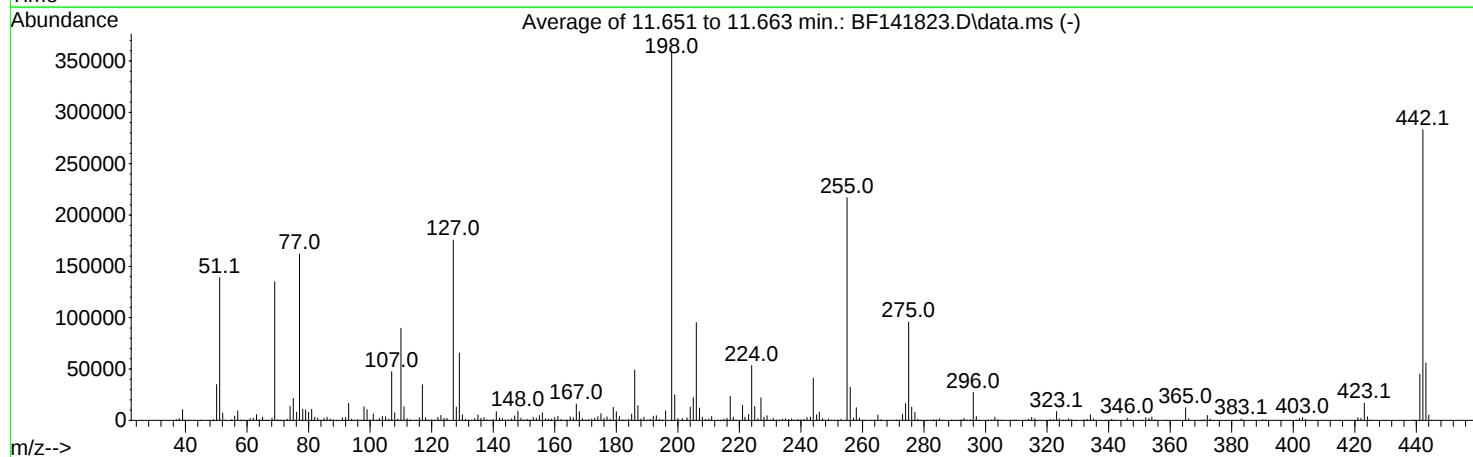


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030425\
Data File : BF141823.D
Acq On : 04 Mar 2025 13:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 28 01:48:16 2025

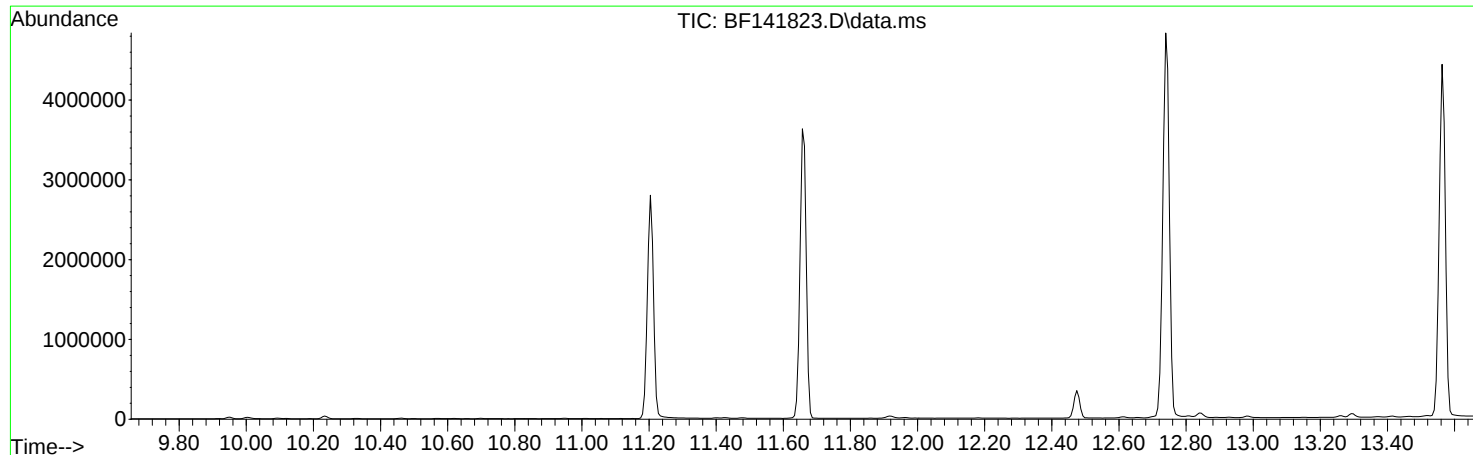

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	139000	PASS
68	69	0.00	2	1.7	2230	PASS
69	198	0.00	100	37.7	134917	PASS
70	69	0.00	2	0.4	560	PASS
127	198	10	80	49.0	175467	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	358293	PASS
199	198	5	9	7.0	25051	PASS
275	198	10	60	26.7	95629	PASS
365	198	1	100	3.5	12382	PASS
441	198	0.01	100	12.5	44824	PASS
442	442	50	100	100.0	283093	PASS
443	442	15	24	19.8	56016	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/4/2025	BNA_F	<u>BF141823.D</u>
Compound Name	Response	Retention Time
DDT	1022885	13.563
DDD	14087	13.292
DDE	897	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14984	1037869	1.44

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030425\
Data File : BF141823.D
Acq On : 04 Mar 2025 13:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 04 14:52:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

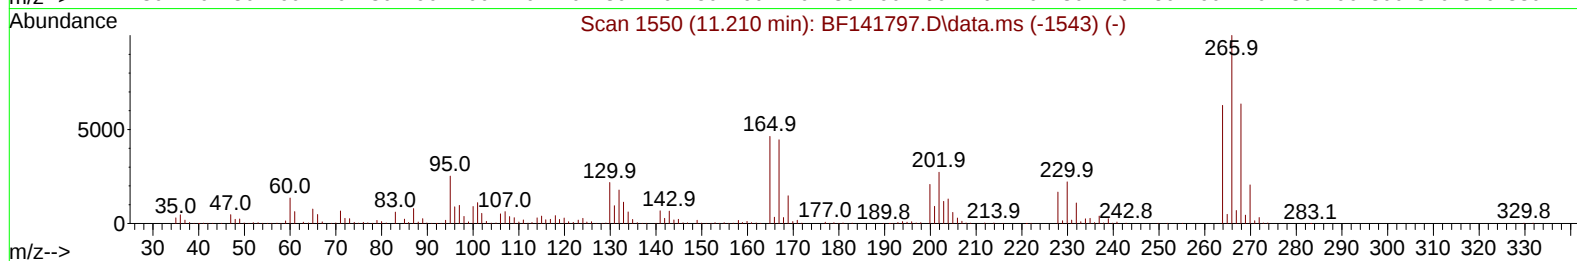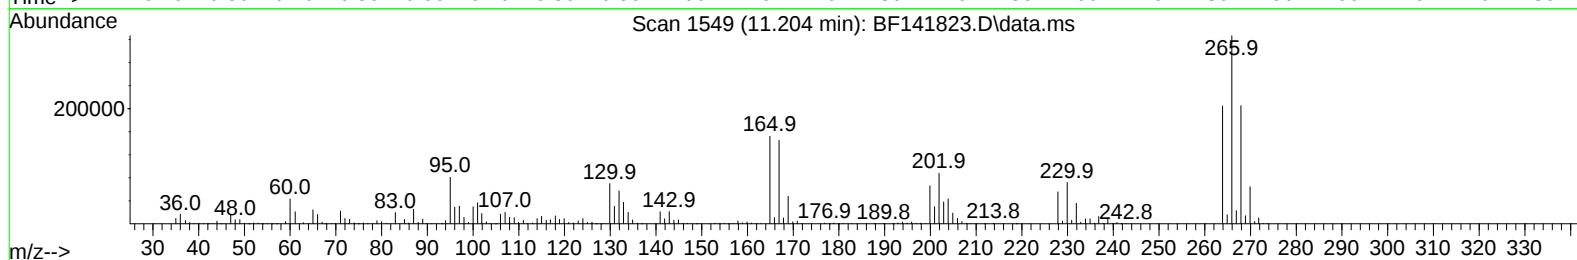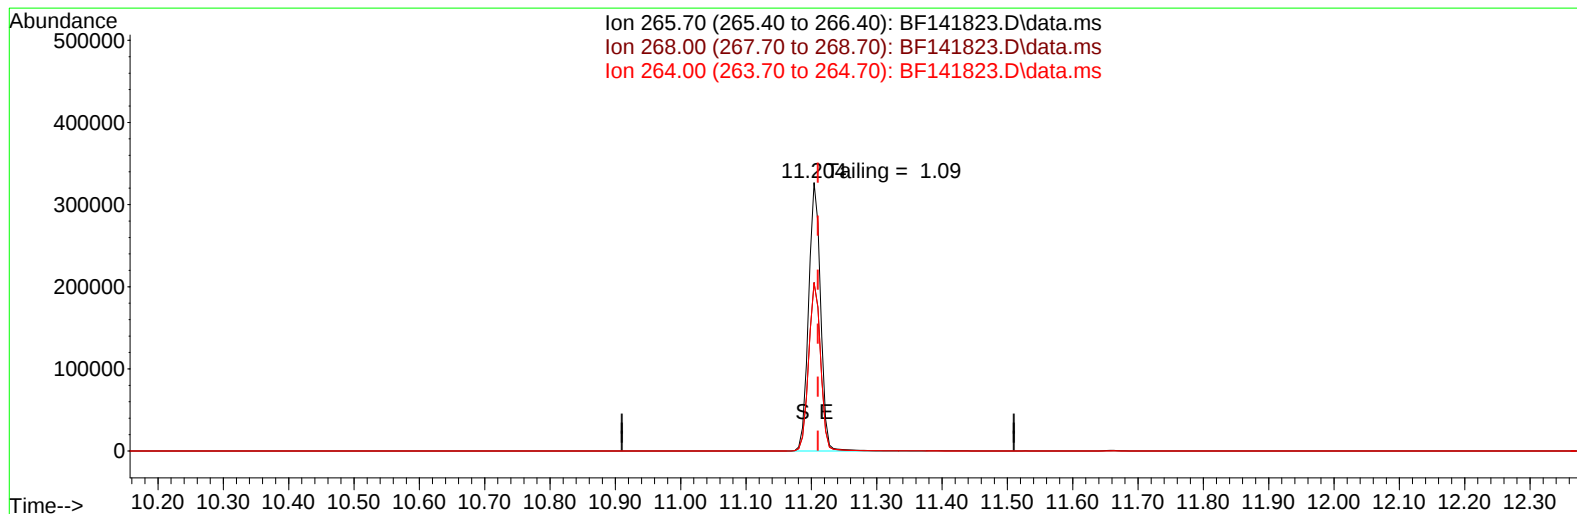

TIC: BF141823.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 15423.04 ng




response 419020

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	62.81
264.00	62.80	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030425\
Data File : BF141823.D
Acq On : 04 Mar 2025 13:16
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 04 14:52:08 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 28 01:48:16 2025
Response via : Initial Calibration

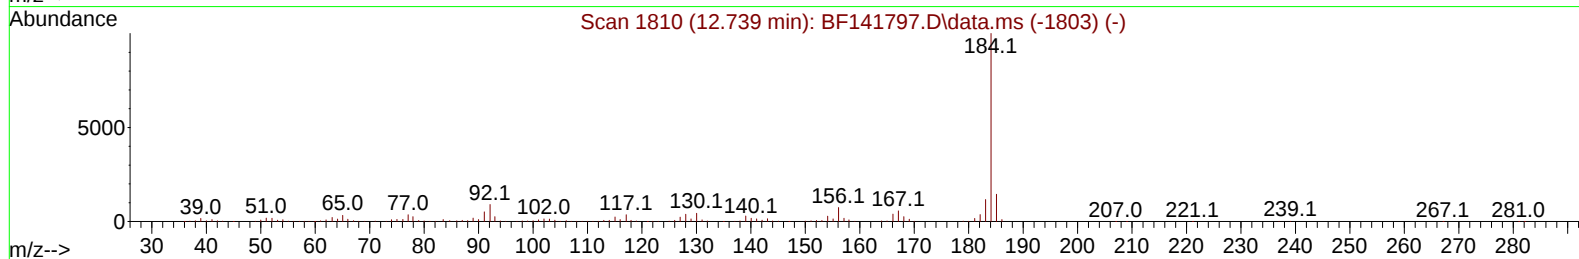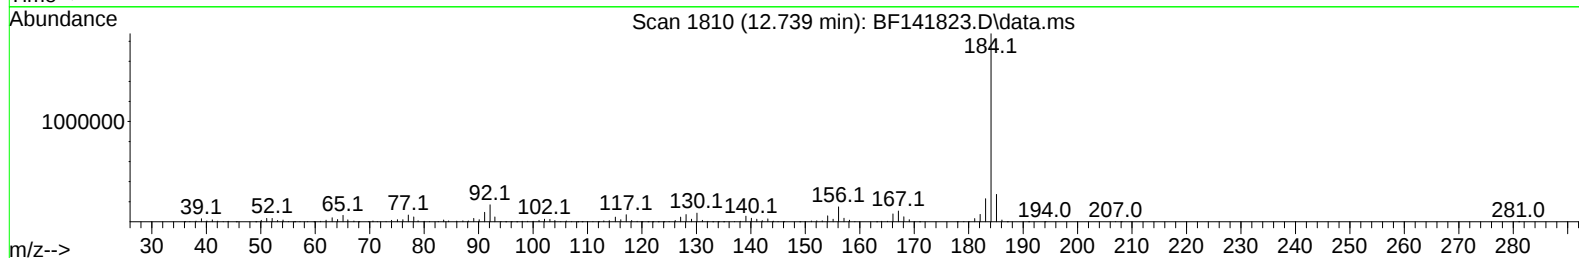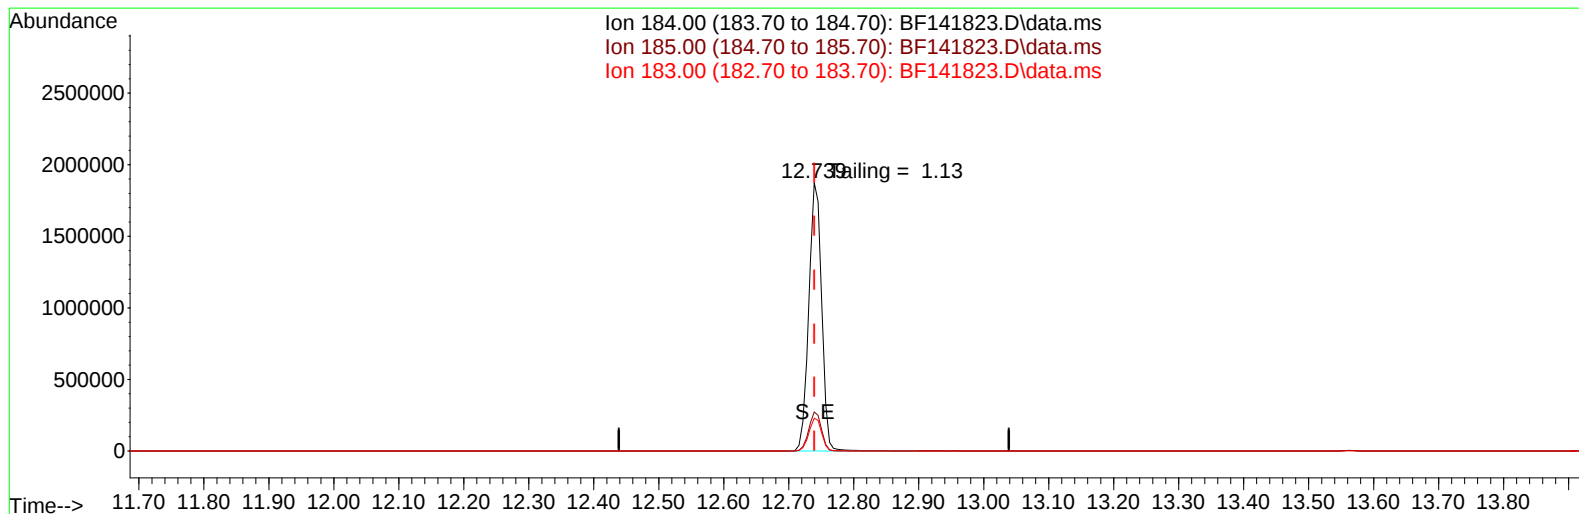

TIC: BF141823.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 62740.05 ng

response 2583016

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.56
183.00	11.70	12.26
0.00	0.00	0.00