

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030518\
 Data File : BF103406.D
 Acq On : 5 Mar 2018 13:43
 Operator : SJ/JU
 Sample : J1751-07 2X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Mar 05 15:12:50 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 05 13:40:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	137015	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	581027	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	255887	20.00	ng	0.00
63) Phenanthrene-d10	11.41	188	404779	20.00	ng	0.00
75) Chrysene-d12	14.07	240	252797	20.00	ng	0.00
86) Perylene-d12	15.58	264	228631	20.00	ng	0.00

System Monitoring Compounds

5) 2-Fluorophenol	5.50	112	437654	48.31	ng	0.00
7) Phenol-d6	6.51	99	546233	49.28	ng	-0.01
23) Nitrobenzene-d5	7.43	82	322545	31.70	ng	0.00
41) 2,4,6-Tribromophenol	10.71	330	81022	37.41	ng	0.00
44) 2-Fluorobiphenyl	9.23	172	476792	26.27	ng	0.00
78) Terphenyl-d14	12.99	244	336893	32.04	ng	0.00

Target Compounds


						Qvalue
9) Benzaldehyde	6.42	77	498	Below Cal	#	1
25) Isophorone	7.43	82	322545	16.097 ng	#	64
37) 2-Methylnaphthalene	8.87	142	46762	2.544 ng		98
49) Dimethylphthalate	9.62	163	149940	7.304 ng		99
51) Acenaphthene	9.95	154	125378	8.238 ng		98
53) 2,4-Dinitrophenol	10.27	184	115	9.686 ng	#	47
54) Dibenzofuran	10.12	168	178922	8.564 ng		98
57) Fluorene	10.46	166	242392	13.620 ng		100
64) 4,6-Dinitro-2-methylphenol	10.70	198	259	5.040 ng	#	1
70) Phenanthrene	11.44	178	1137860	51.080 ng		99
71) Anthracene	11.49	178	481987	21.100 ng		100
72) Carbazole	11.64	167	95301	4.189 ng		99
74) Fluoranthene	12.63	202	1167123	52.138 ng		98
77) Pyrene	12.86	202	999290	50.701 ng		100
80) Benzo(a)anthracene	14.06	228	513932	31.333 ng		99
82) Chrysene	14.09	228	396517	24.897 ng		98
85) Indeno(1,2,3-cd)pyrene	17.13	276	139810	11.089 ng		97
87) Benzo(b)fluoranthene	15.14	252	613097	40.785 ng	#	94
88) Benzo(k)fluoranthene	15.14	252	613097	43.312 ng	#	97
89) Benzo(a)pyrene	15.52	252	316817	23.601 ng		96
90) Dibenzo(a,h)anthracene	17.13	278	38581	3.719 ng	#	77
91) Benzo(g,h,i)perylene	17.60	276	128180	12.644 ng		97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030518\
Data File : BF103406.D
Acq On : 5 Mar 2018 13:43
Operator : SJ/JU
Sample : J1751-07 2X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Mar 05 15:12:50 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 05 13:40:47 2018
Response via : Initial Calibration

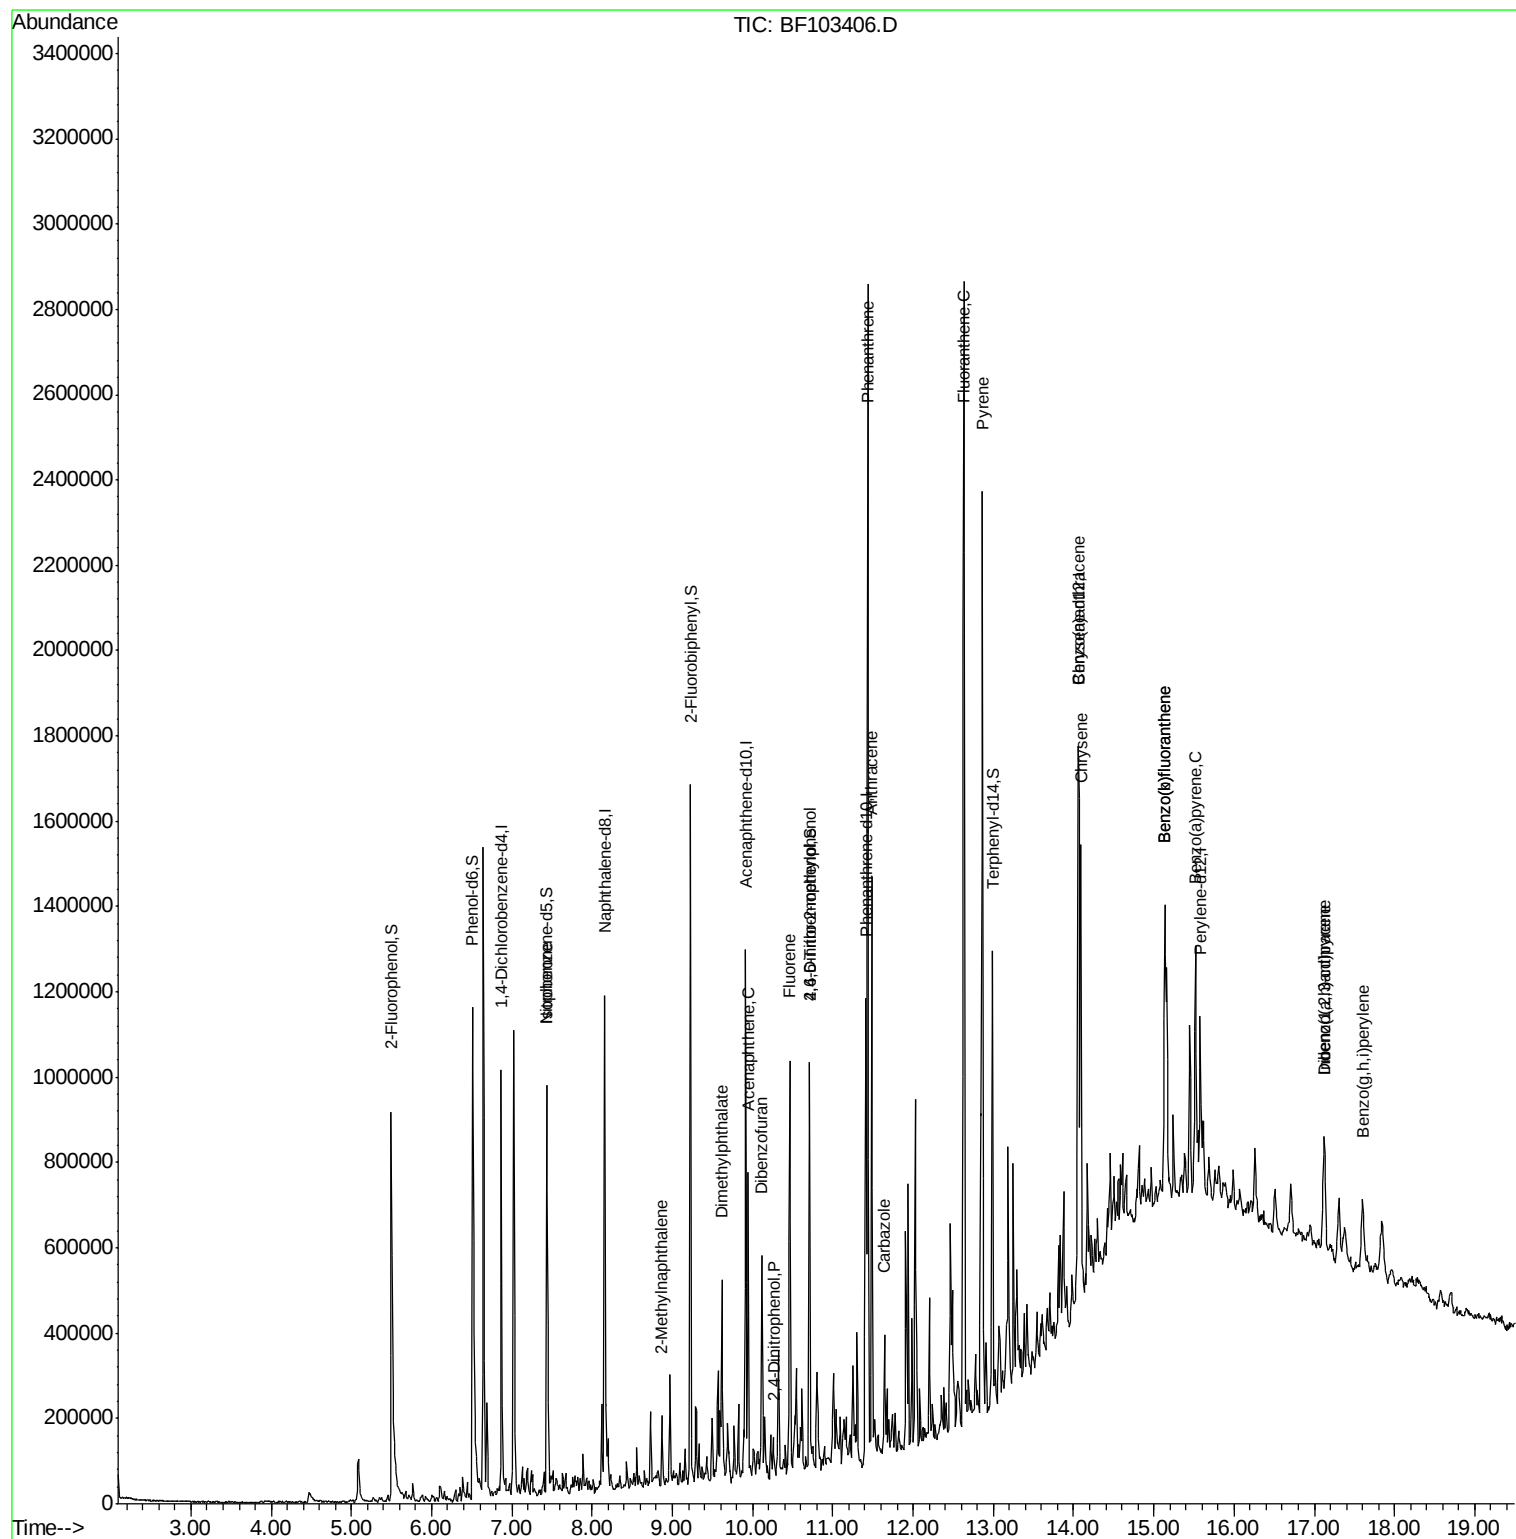




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.87 min Scan# 813
Delta R.T. -0.00 min
Lab File: BF103406.D
Acq: 5 Mar 2018 13:43

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 137015
Ion Ratio Lower Upper
152 100
150 158.0 124.6 186.8
115 67.0 50.1 75.1

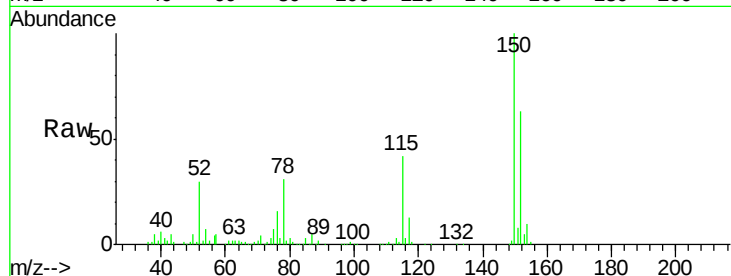


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

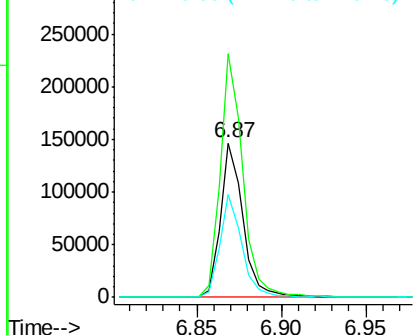



#5


2-Fluorophenol
Concen: 48.310 ng
RT: 5.50 min Scan# 581
Delta R.T. -0.00 min
Lab File: BF103406.D
Acq: 5 Mar 2018 13:43

Tgt Ion:112 Resp: 437654
Ion Ratio Lower Upper
112 100
64 63.8 47.9 71.9
63 34.1 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

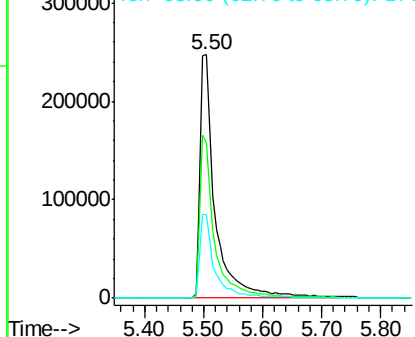

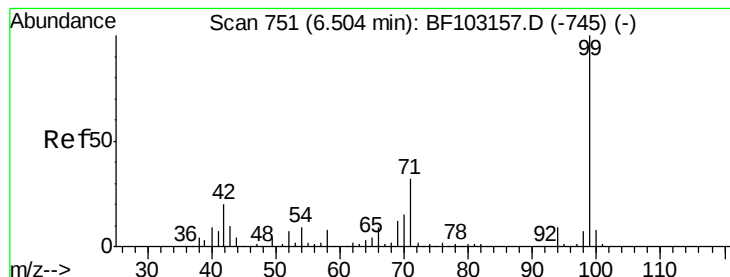

#7

Phenol-d6

Concen: 49.275 ng

RT: 6.51 min Scan# 752

Delta R.T. -0.01 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43


Instrument :

BNA_F

ClientSampled :

Tot Ion: 99 Resp: 546233




Ion	Ratio	Lower	Upper
99	100		
42	22.7	14.5	21.7#
71	33.4	25.4	38.0



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

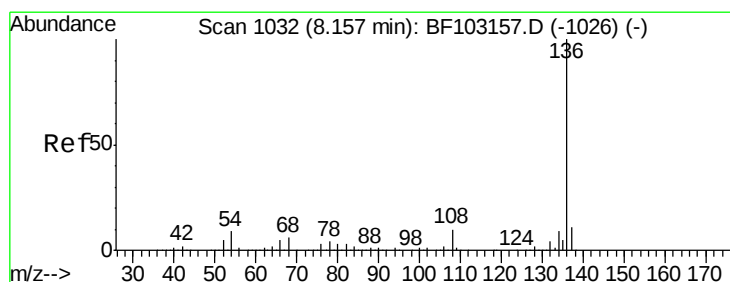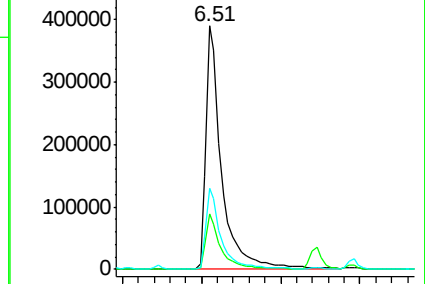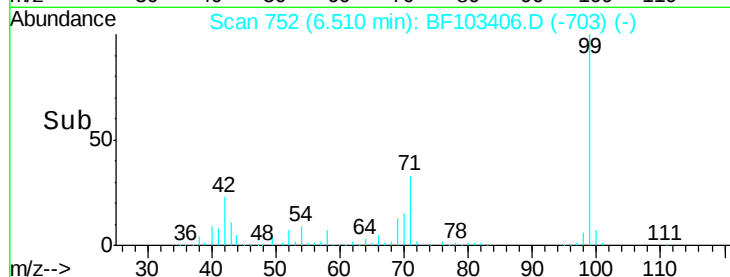

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1032


Delta R.T. -0.00 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43

Tgt Ion: 136 Resp: 581027

Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	8.5	6.6	9.8
68	6.3	5.0	7.4


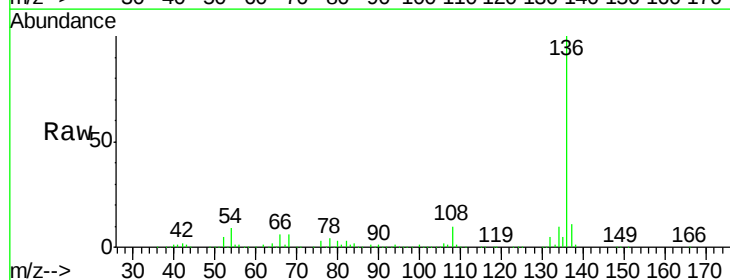



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



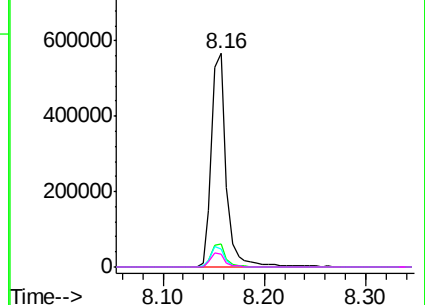
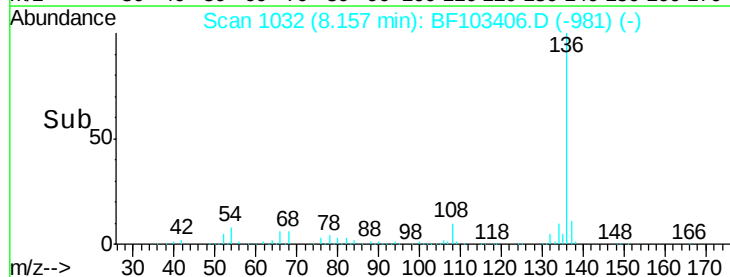




#23
Nitrobenzene-d5
Concen: 31.703 ng
RT: 7.43 min Scan# 909
Delta R.T. -0.01 min
Lab File: BF103406.D
Acq: 5 Mar 2018 13:43




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 82 Resp: 322545
Ion Ratio Lower Upper
82 100
128 41.2 36.1 54.1
54 61.5 41.4 62.2

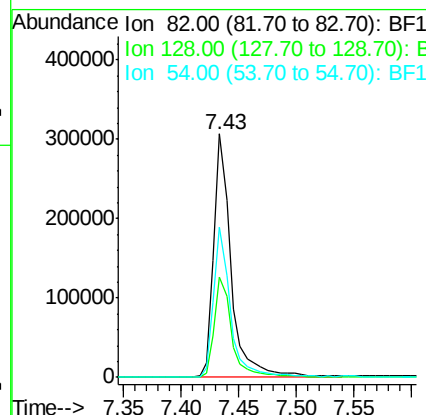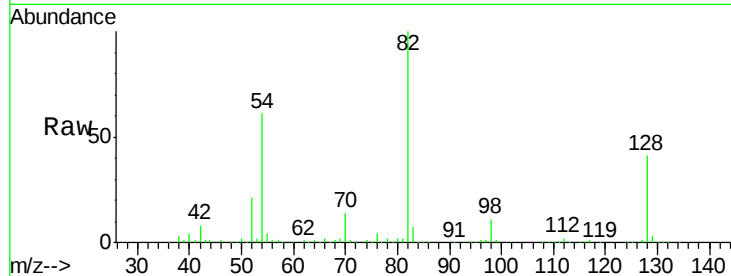

#25
Isophorone
Concen: 16.097 ng
RT: 7.43 min Scan# 909
Delta R.T. -0.26 min
Lab File: BF103406.D
Acq: 5 Mar 2018 13:43

Tgt Ion: 82 Resp: 322545
Ion Ratio Lower Upper
82 100
95 0.3 5.2 7.8#
138 0.0 14.9 22.3#



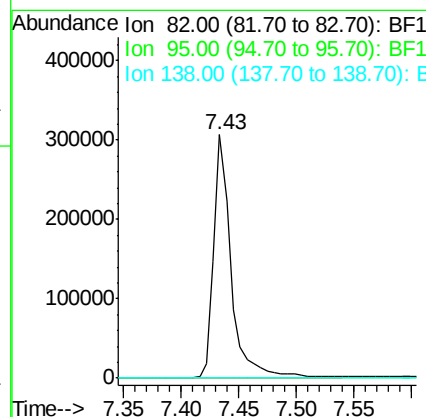



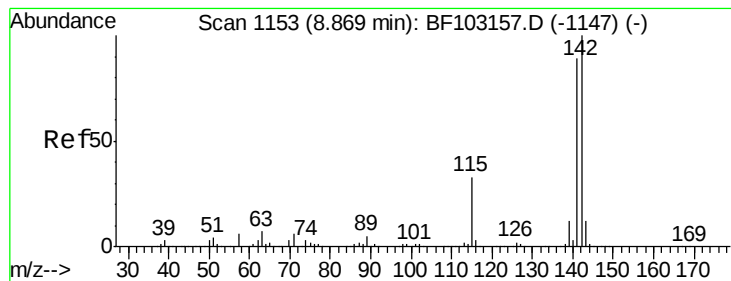

#37
 2-Methylnaphthalene
 Concen: 2.544 ng
 RT: 8.87 min Scan# 1153
 Delta R.T. -0.00 min
 Lab File: BF103406.D
 Acq: 5 Mar 2018 13:43




Instrument :
 BNA_F
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
142	100		
141	90.8	70.8	106.2
115	33.4	26.1	39.1

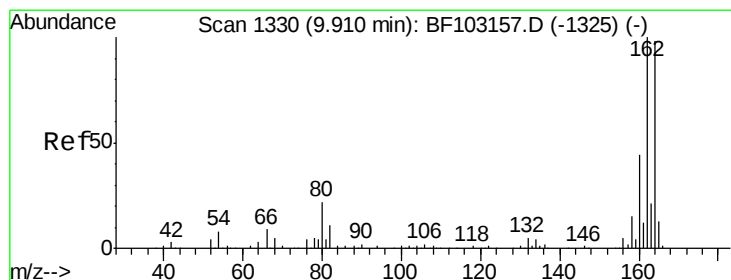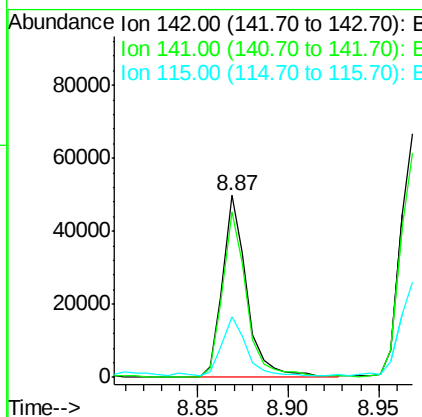

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.00 min
 Lab File: BF103406.D
 Acq: 5 Mar 2018 13:43

Tgt Ion	Ratio	Lower	Upper
164	100		
162	103.1	86.1	129.1
160	47.0	38.3	57.5

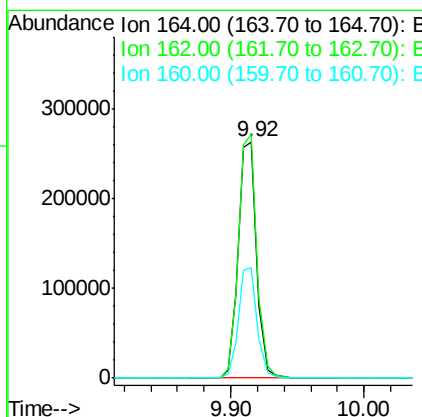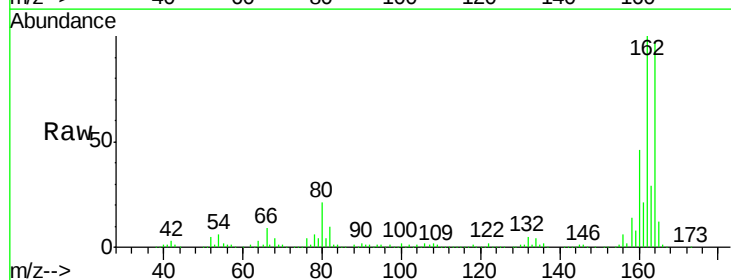


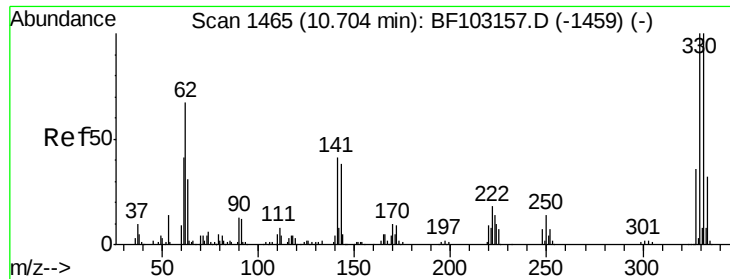




#41
 2,4,6-Tribromophenol
 Concen: 37.407 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. -0.01 min
 Lab File: BF103406.D
 Acq: 5 Mar 2018 13:43

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 81022
 Ion Ratio Lower Upper
 330 100
 332 105.2 77.0 115.6
 141 49.9 29.9 44.9#

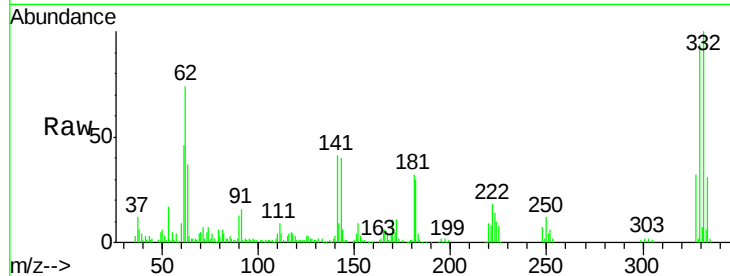


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

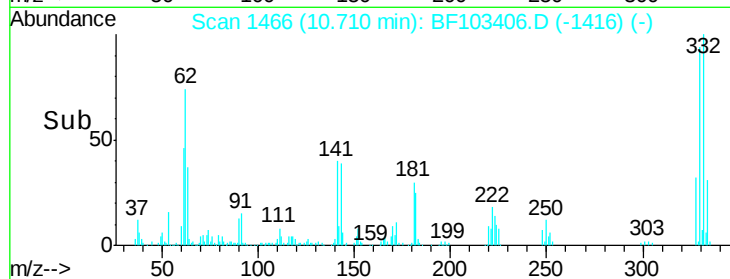
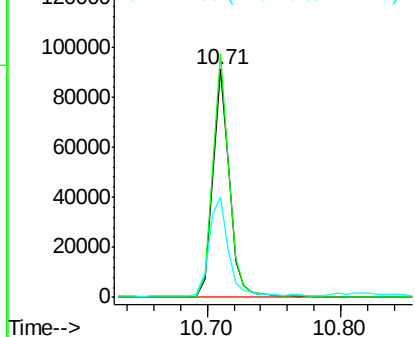



#44
 2-Fluorobiphenyl
 Concen: 26.270 ng
 RT: 9.23 min Scan# 1214
 Delta R.T. -0.01 min
 Lab File: BF103406.D
 Acq: 5 Mar 2018 13:43

Tgt Ion:172 Resp: 476792
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.7 44.5
 170 24.2 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

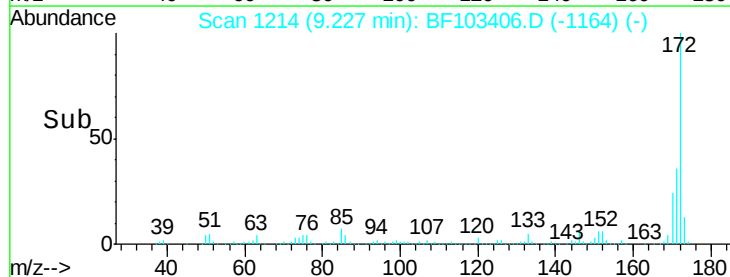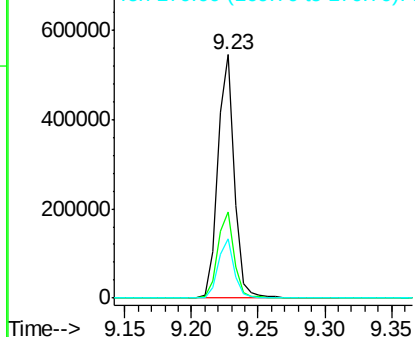


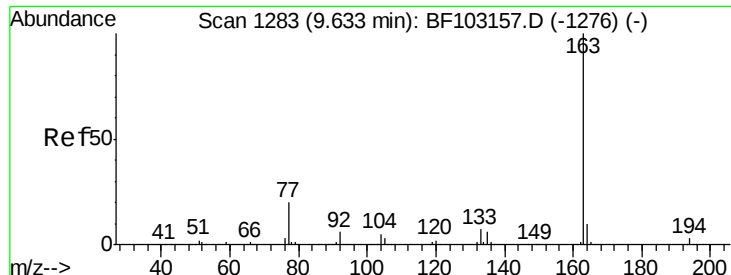




#49
Dimethylphthalate
Concen: 7.304 ng
RT: 9.62 min Scan# 1281
Delta R.T. -0.01 min
Lab File: BF103406.D
Acq: 5 Mar 2018 13:43

Instrument :
BNA_F
ClientSampleId :

Tot Ion:163 Resp: 149940
Ion Ratio Lower Upper
163 100
194 3.3 2.7 4.1
164 9.7 8.2 12.2

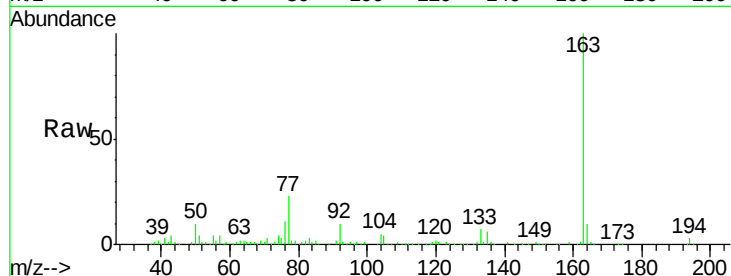


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E


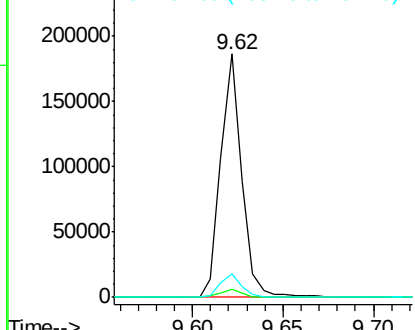



#51
Acenaphthene
Concen: 8.238 ng
RT: 9.95 min Scan# 1336
Delta R.T. -0.01 min
Lab File: BF103406.D
Acq: 5 Mar 2018 13:43

Tgt Ion:154 Resp: 125378
Ion Ratio Lower Upper
154 100
153 112.1 91.2 136.8
152 55.9 43.8 65.8



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E



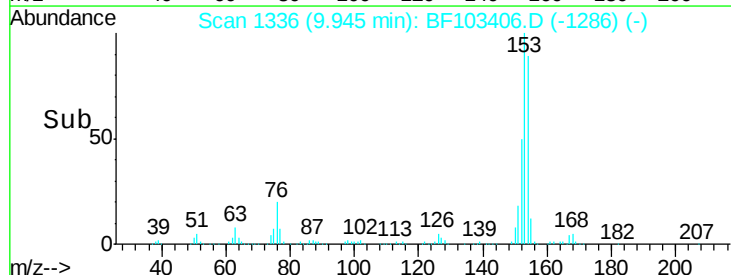
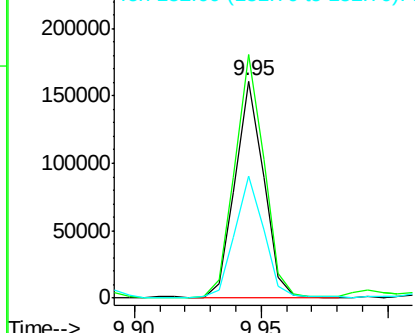




#53
 2,4-Dinitrophenol
 Concen: 9.686 ng
 RT: 10.27 min Scan# 1392
 Delta R.T. 0.27 min
 Lab File: BF103406.D
 Acq: 5 Mar 2018 13:43




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:184 Resp: 115
 Ion Ratio Lower Upper
 184 100
 63 96.3 54.2 81.2#
 154 133.2 184.0 276.0#

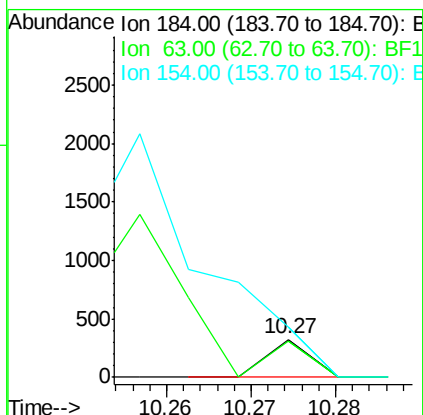

#54
 Dibenzofuran
 Concen: 8.564 ng
 RT: 10.12 min Scan# 1366
 Delta R.T. -0.00 min
 Lab File: BF103406.D
 Acq: 5 Mar 2018 13:43

Tgt Ion:168 Resp: 178922
 Ion Ratio Lower Upper
 168 100
 139 38.8 30.1 45.1
 169 13.4 10.9 16.3



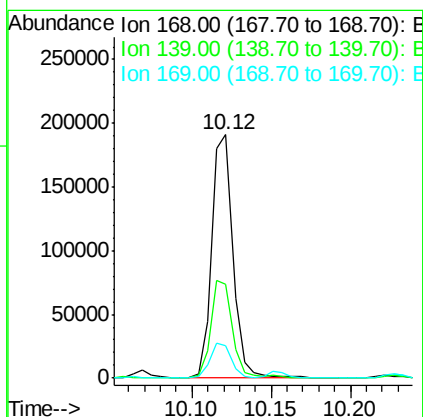





#57
Fluorene
 Concen: 13.620 ng
 RT: 10.46 min Scan# 1424
 Delta R.T. -0.01 min
 Lab File: BF103406.D
 Acq: 5 Mar 2018 13:43




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
166	100		
165	99.7	79.8	119.8
167	14.0	10.6	16.0

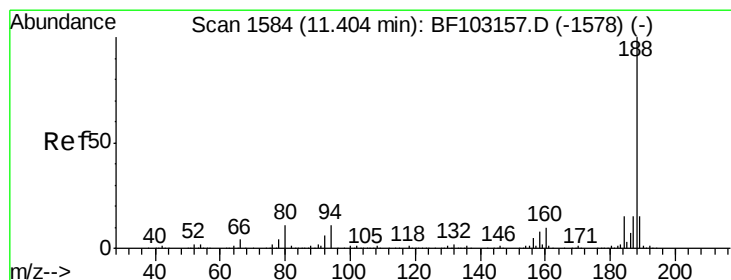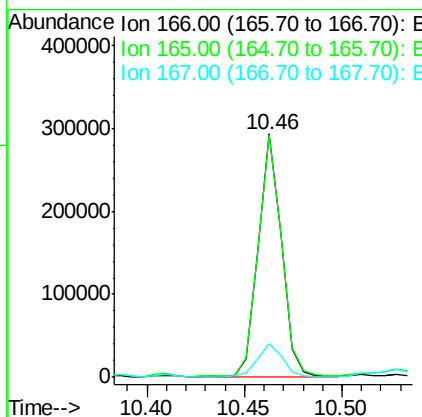

#63
Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.41 min Scan# 1585
 Delta R.T. -0.00 min
 Lab File: BF103406.D
 Acq: 5 Mar 2018 13:43

Tgt Ion	Ratio	Lower	Upper
188	100		
94	10.6	8.5	12.7
80	11.6	9.2	13.8

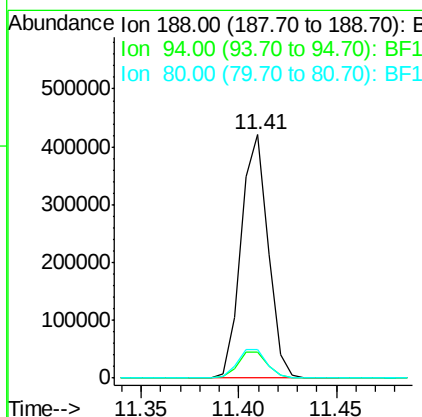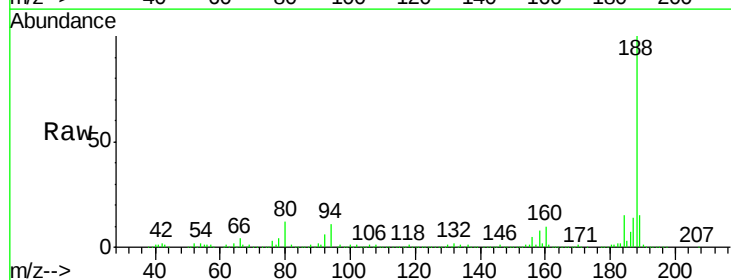



#64

4,6-Dinitro-2-methylphenol

Concen: 5.040 ng

RT: 10.70 min Scan# 1465

Delta R.T. 0.17 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43

Instrument :

BNA_F

ClientSampleId :


Tot Ion:198 Resp: 259

Ion Ratio Lower Upper

198 100

51 793.0 37.7 77.7#




105 253.4 36.3 76.3#

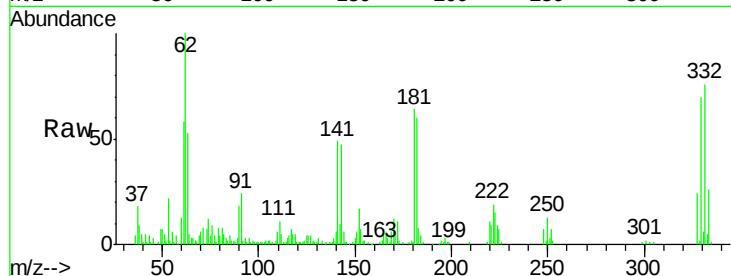

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BF1

Ion 105.00 (104.70 to 105.70): E

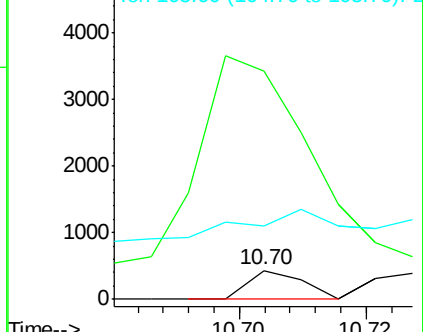

#70

Phenanthrene

Concen: 51.080 ng

RT: 11.44 min Scan# 1590

Delta R.T. 0.01 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43


Tgt Ion:178 Resp: 1137860

Ion Ratio Lower Upper

178 100

176 20.4 15.8 23.8



179 15.8 13.0 19.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

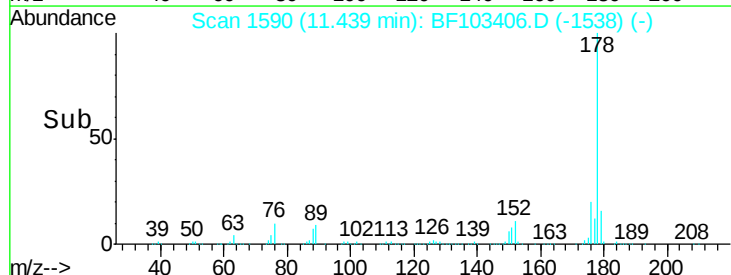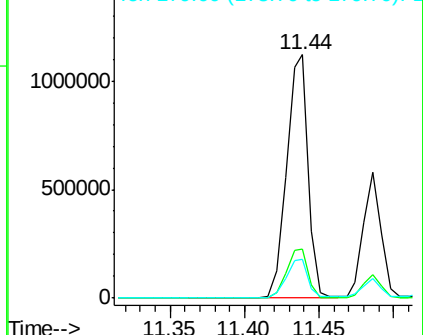


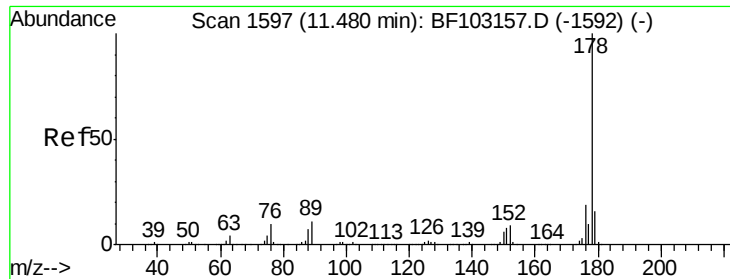




#71
 Anthracene
 Concen: 21.100 ng
 RT: 11.49 min Scan# 1598
 Delta R.T. -0.00 min
 Lab File: BF103406.D
 Acq: 5 Mar 2018 13:43

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:178 Resp: 481987
 Ion Ratio Lower Upper
 178 100
 176 19.2 15.4 23.2
 179 15.5 12.6 19.0




Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E

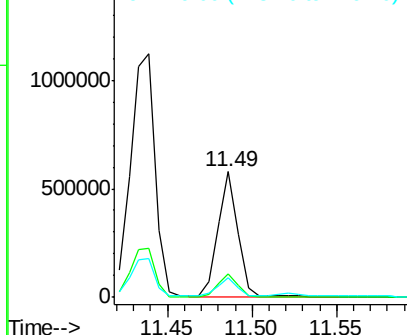
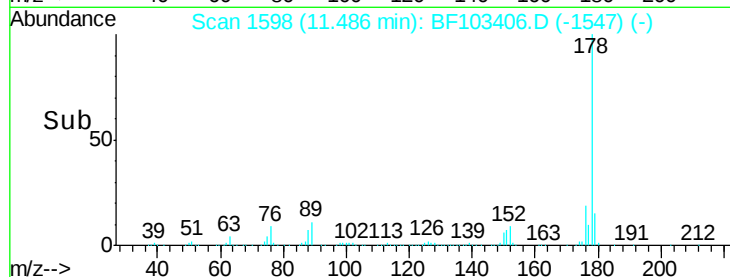



#72
 Carbazole
 Concen: 4.189 ng
 RT: 11.64 min Scan# 1625
 Delta R.T. -0.01 min
 Lab File: BF103406.D
 Acq: 5 Mar 2018 13:43

Tgt Ion:167 Resp: 95301
 Ion Ratio Lower Upper
 167 100
 166 22.1 17.6 26.4
 139 14.6 10.9 16.3



Abundance Ion 167.00 (166.70 to 167.70): E
 Ion 166.00 (165.70 to 166.70): E
 Ion 139.00 (138.70 to 139.70): E

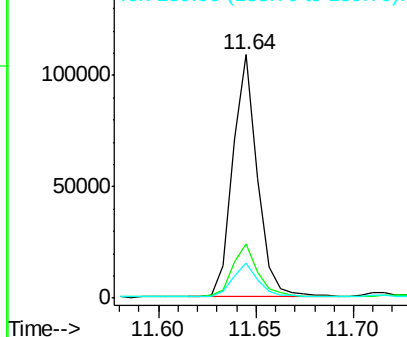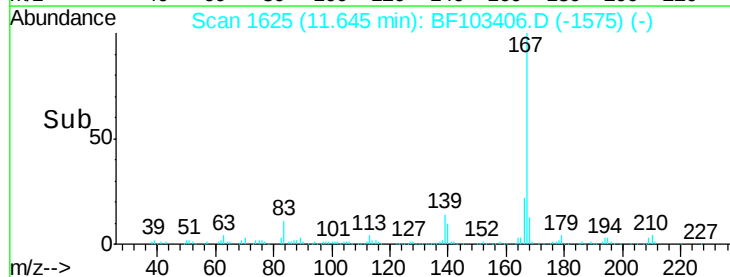

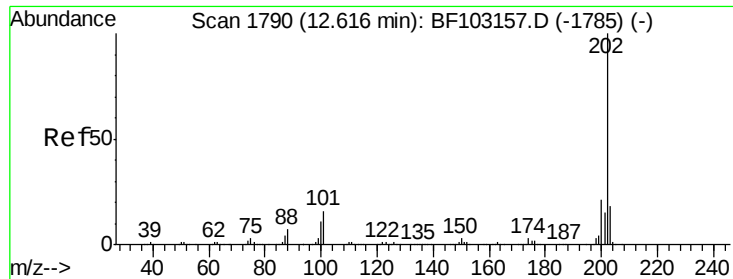

#74

Fluoranthene

Concen: 52.138 ng

RT: 12.63 min Scan# 1793

Delta R.T. -0.00 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43

Instrument :

BNA_F

ClientSampleId :


Tot Ion:202 Resp: 1167123

Ion Ratio Lower Upper

202 100

101 15.9 0.0 34.1




203 17.9 0.0 38.1

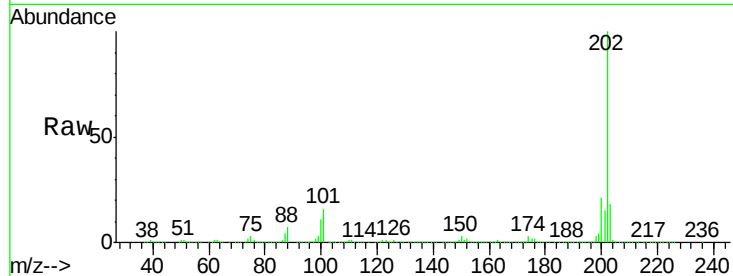

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

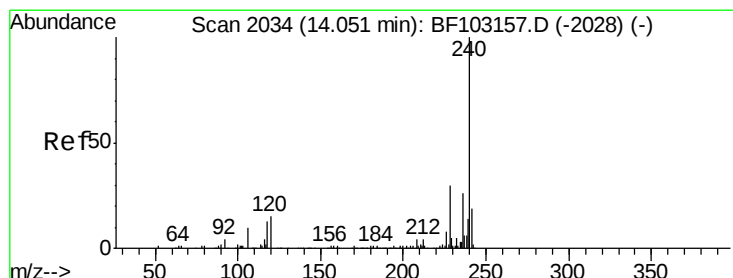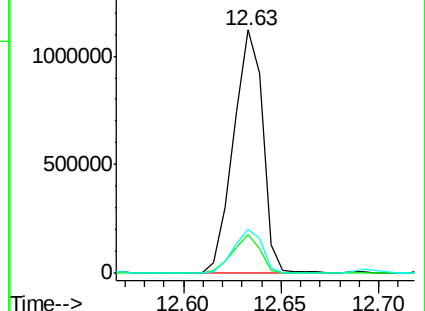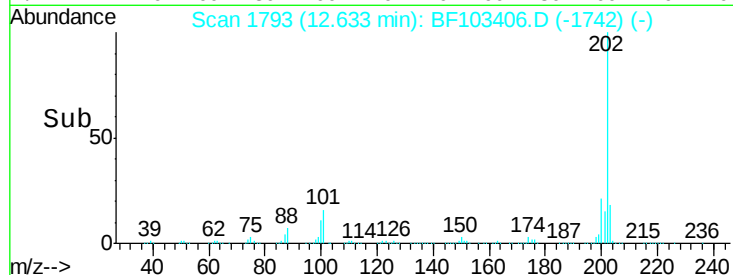

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.07 min Scan# 2037

Delta R.T. -0.00 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43


Tgt Ion:240 Resp: 252797

Ion Ratio Lower Upper

240 100

120 13.9 9.5 14.3



236 27.0 20.7 31.1

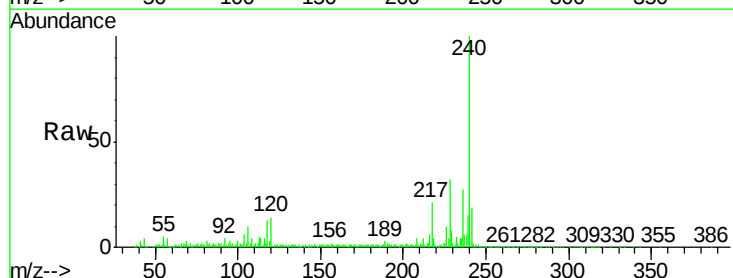


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

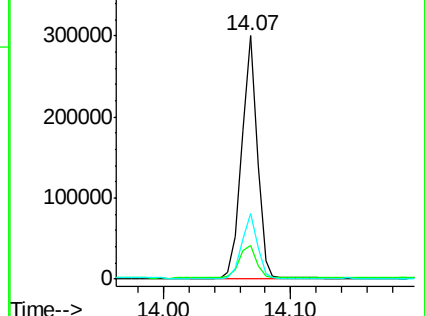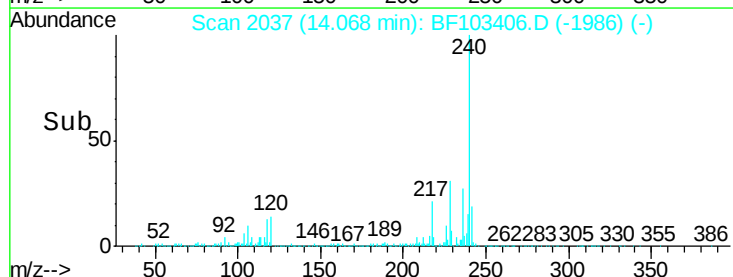

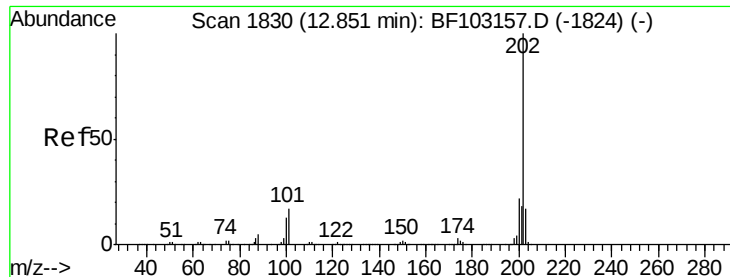

#77

Pvrene

Concen: 50.701 ng

RT: 12.86 min Scan# 1832

Delta R.T. -0.00 min

Lab File: BF103406.D





Acq: 5 Mar 2018 13:43

Instrument :

BNA_F

ClientSampleId :

Tot Ion:	202	Resp:	999290
Ion	Ratio	Lower	Upper
202	100		
200	21.8	17.4	26.2
203	18.2	14.3	21.5

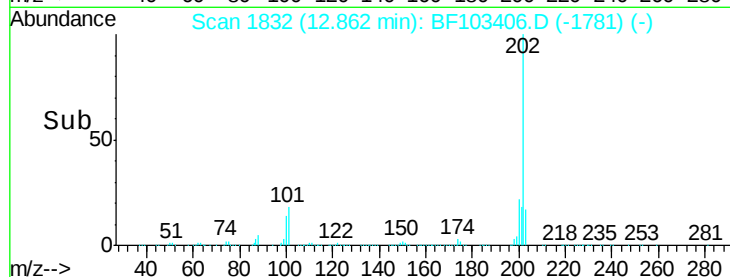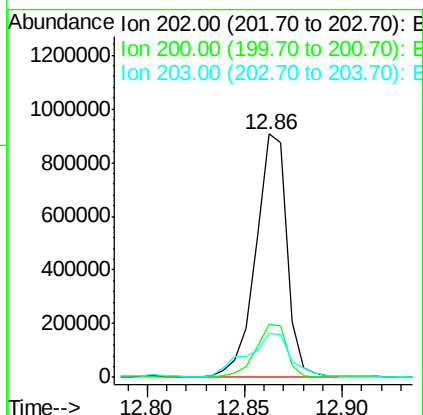

#78

Terphenyl-d14

Concen: 32.035 ng




RT: 12.99 min Scan# 1854


Delta R.T. -0.00 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43

Tgt Ion:	244	Resp:	336893
Ion	Ratio	Lower	Upper
244	100		
212	7.2	5.4	8.0
122	13.0	11.0	16.4


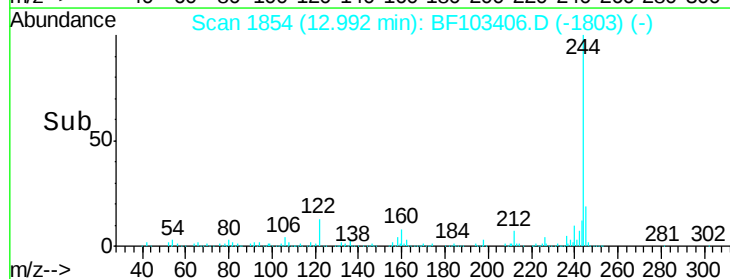
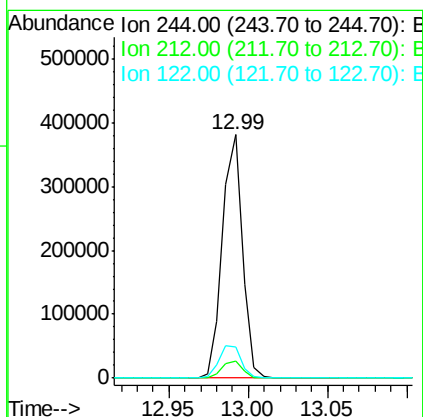





#80
Benzo(a)anthracene
Concen: 31.333 ng
RT: 14.06 min Scan# 2035
Delta R.T. -0.00 min
Lab File: BF103406.D
Acq: 5 Mar 2018 13:43




Instrument :
BNA_F
ClientSampleId :


Tot Ion:228 Resp: 513932
Ion Ratio Lower Upper
228 100
226 27.7 22.6 33.8
229 20.2 15.8 23.6

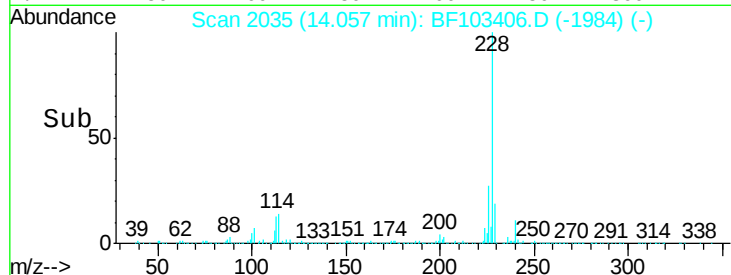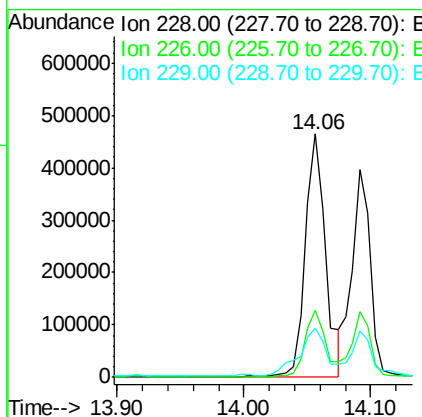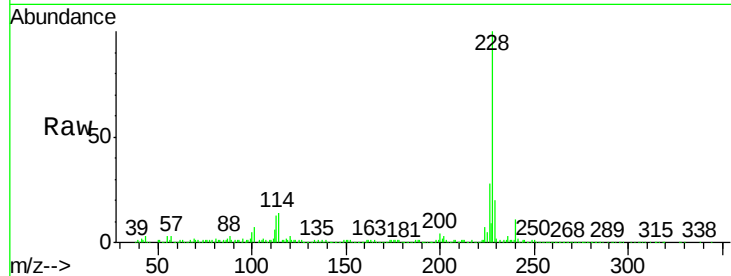

#82
Chrysene
Concen: 24.897 ng
RT: 14.09 min Scan# 2041
Delta R.T. -0.01 min
Lab File: BF103406.D
Acq: 5 Mar 2018 13:43

Tgt Ion:228 Resp: 396517
Ion Ratio Lower Upper
228 100
226 31.6 25.0 37.6
229 22.5 16.2 24.4

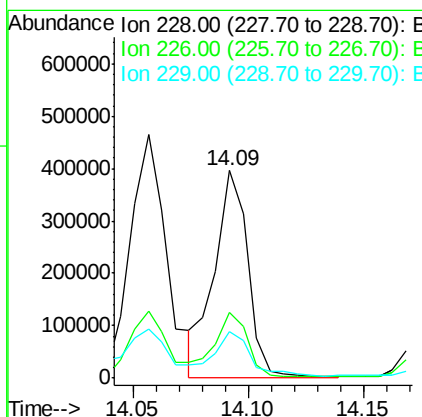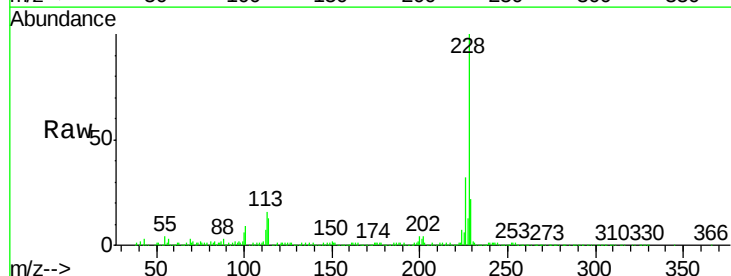



#85

Indeno(1,2,3-cd)pyrene

Concen: 11.089 ng

RT: 17.13 min Scan# 2557

Delta R.T. -0.01 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43


Instrument :

BNA_F

ClientSampleId :

Tot Ion:276 Resp: 139810


Ion	Ratio	Lower	Upper
276	100		
138	28.8	25.0	37.6
277	24.2	20.1	30.1

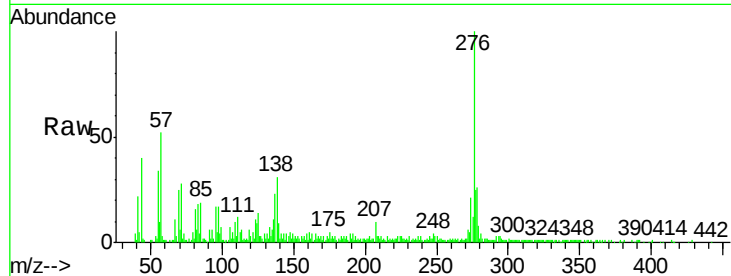


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

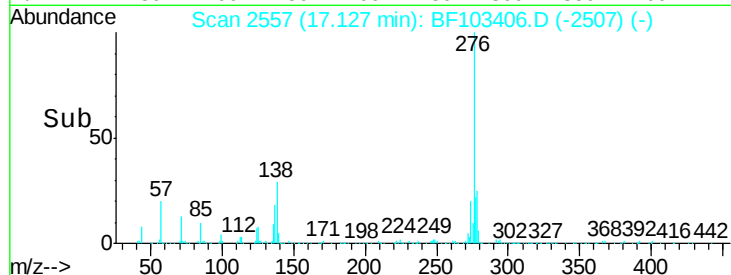

Time-->



#86

Perylene-d12

Concen: 20.000 ng

RT: 15.58 min Scan# 2294


Delta R.T. 0.01 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43

Tgt Ion:264 Resp: 228631


Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.2	28.8
265	23.0	17.5	26.3




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E



Time-->



#87

Benzo(b)fluoranthene

Concen: 40.785 ng

RT: 15.14 min Scan# 2219

Delta R.T. 0.01 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43

Instrument :

BNA_F

ClientSampleId :


Tot Ion:252 Resp: 613097

Ion Ratio Lower Upper

252 100

253 23.1 17.0 25.6




125 15.4 9.0 13.6#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

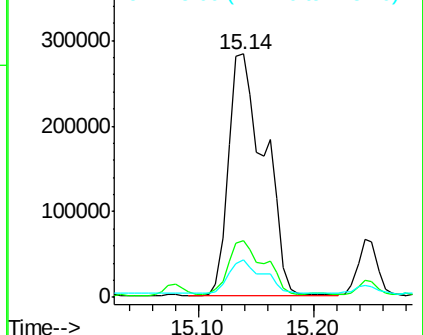

#88

Benzo(k)fluoranthene

Concen: 43.312 ng

RT: 15.14 min Scan# 2219

Delta R.T. -0.02 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43


Tgt Ion:252 Resp: 613097

Ion Ratio Lower Upper

252 100

253 23.1 17.9 26.9



125 15.4 10.2 15.2#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E




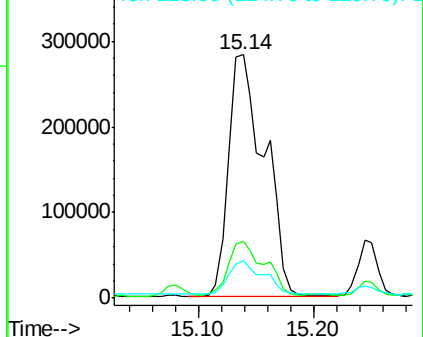


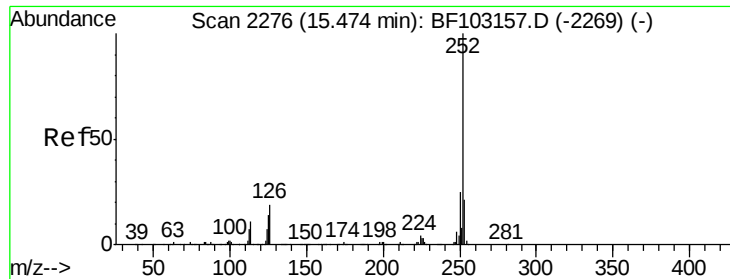

#89
Benzo(a)pyrene
Concen: 23.601 ng
RT: 15.52 min Scan# 2284
Delta R.T. 0.01 min
Lab File: BF103406.D
Acq: 5 Mar 2018 13:43




Instrument :
BNA_F
ClientSampleId :


Tot Ion:252 Resp: 316817
Ion Ratio Lower Upper
252 100
253 22.5 17.1 25.7
125 14.6 9.8 14.6

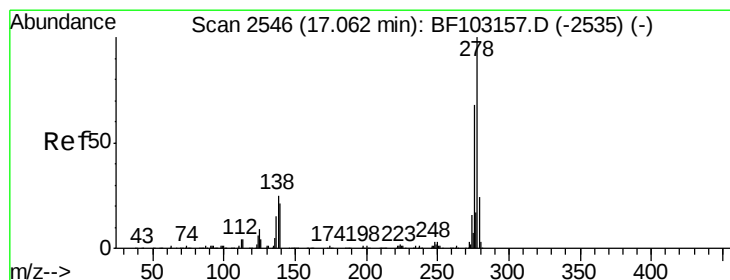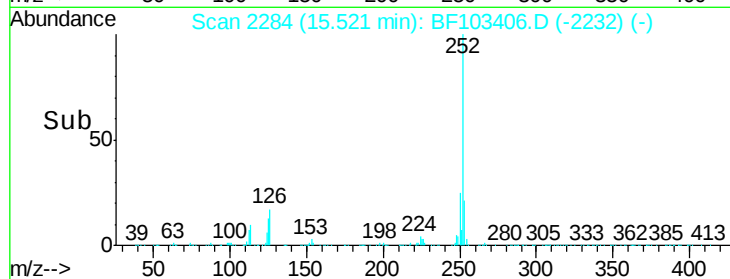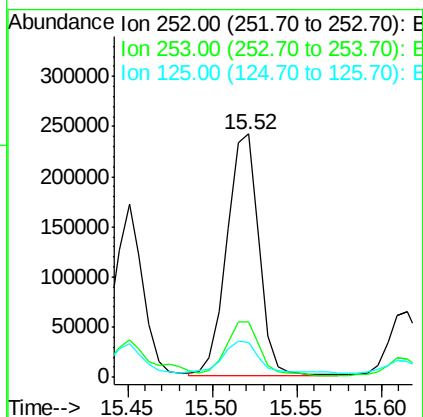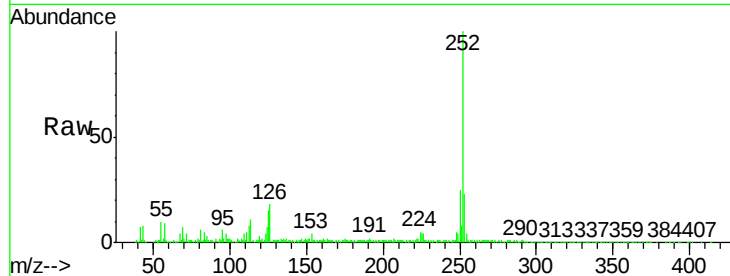

#90
Dibenzo(a,h)anthracene
Concen: 3.719 ng
RT: 17.13 min Scan# 2557
Delta R.T. -0.01 min
Lab File: BF103406.D
Acq: 5 Mar 2018 13:43

Tgt Ion:278 Resp: 38581
Ion Ratio Lower Upper
278 100
139 33.7 15.9 23.9#
279 32.2 19.0 28.4#

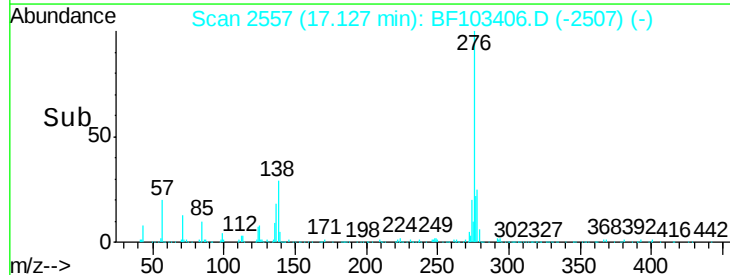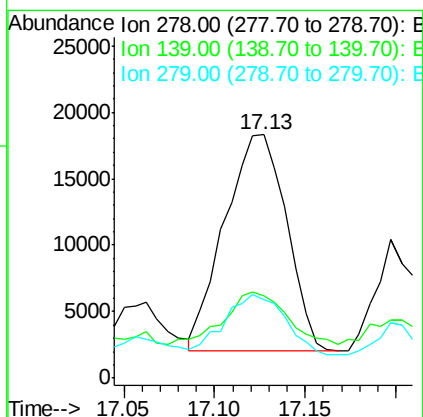



#91

Benzo(a,h,i)perylene

Concen: 12.644 ng

RT: 17.60 min Scan# 2637

Delta R.T. 0.01 min

Lab File: BF103406.D

Acq: 5 Mar 2018 13:43

Instrument :

BNA_F

ClientSampleId :


Tot Ion:276 Resp: 128180

Ion Ratio Lower Upper

276 100

277 23.8 17.9 26.9

138 28.8 21.8 32.8



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

