
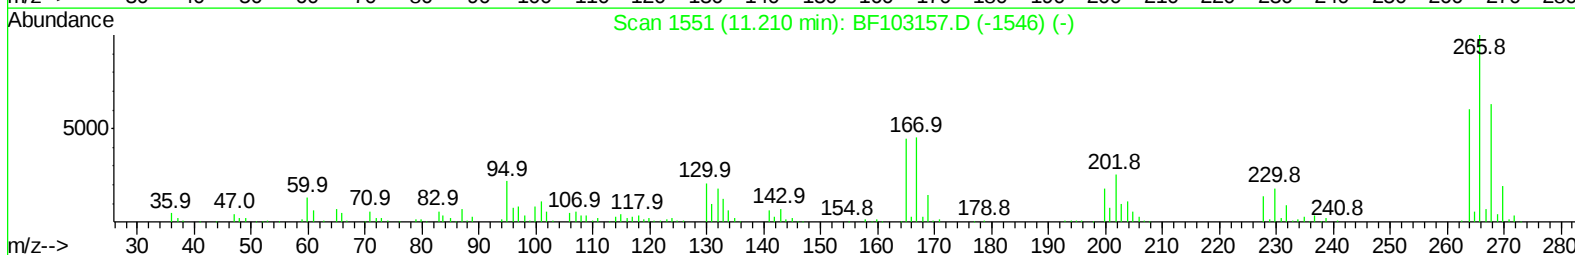
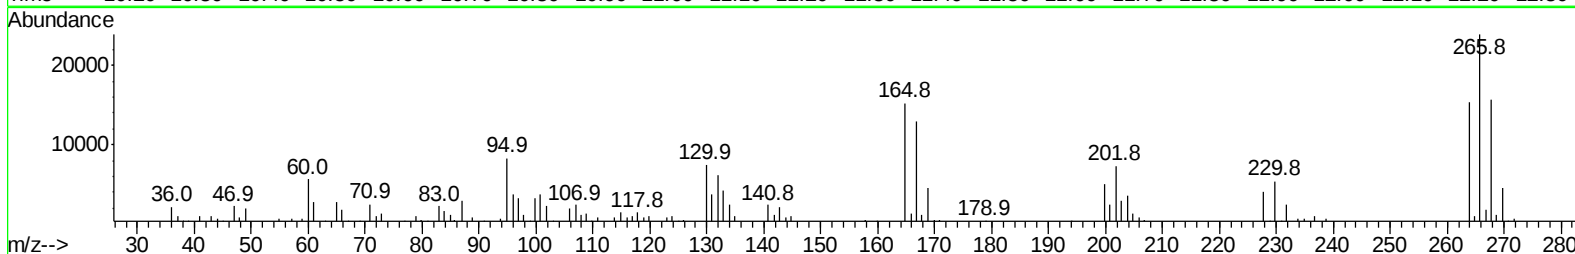


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030518\
Data File : BF103399.D
Acq On : 5 Mar 2018 10:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 06 03:05:42 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 05 13:40:47 2018
Response via : Initial Calibration

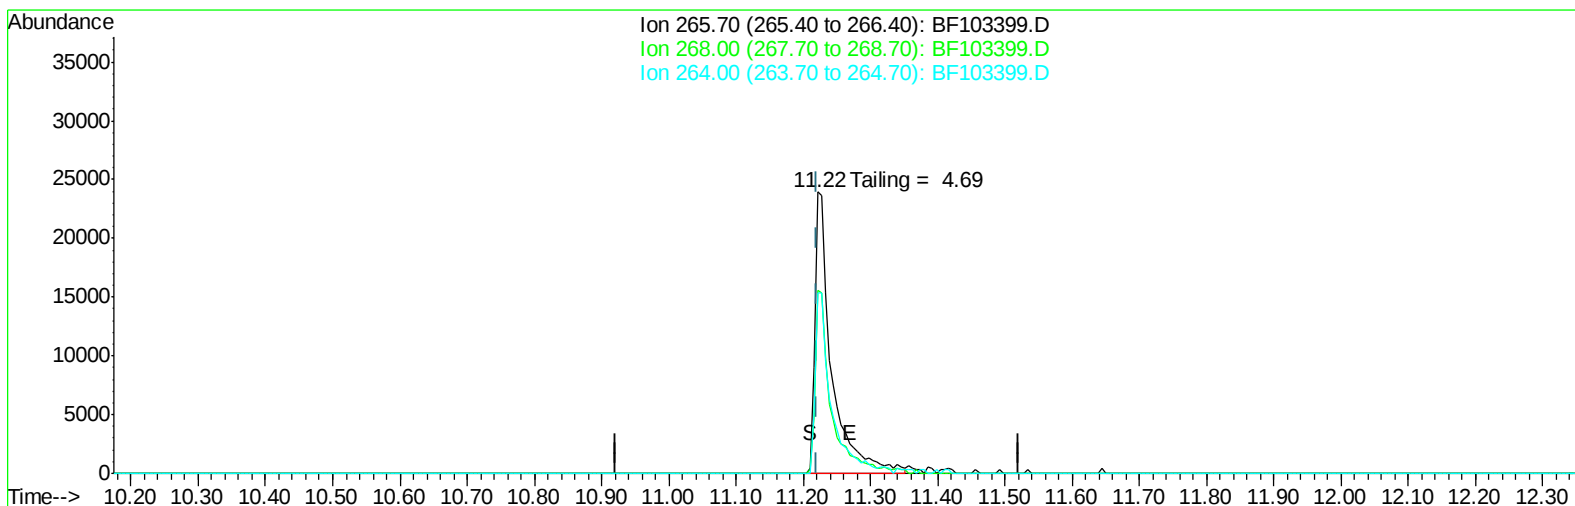

TIC: BF103399.D

(69) Pentachlorophenol (C)




11.221min (-0.000) 51958.36ng

response 42324

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	70.03
264.00	61.90	68.53
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030518\
Data File : BF103399.D
Acq On : 5 Mar 2018 10:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 06 03:05:42 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 05 13:40:47 2018
Response via : Initial Calibration

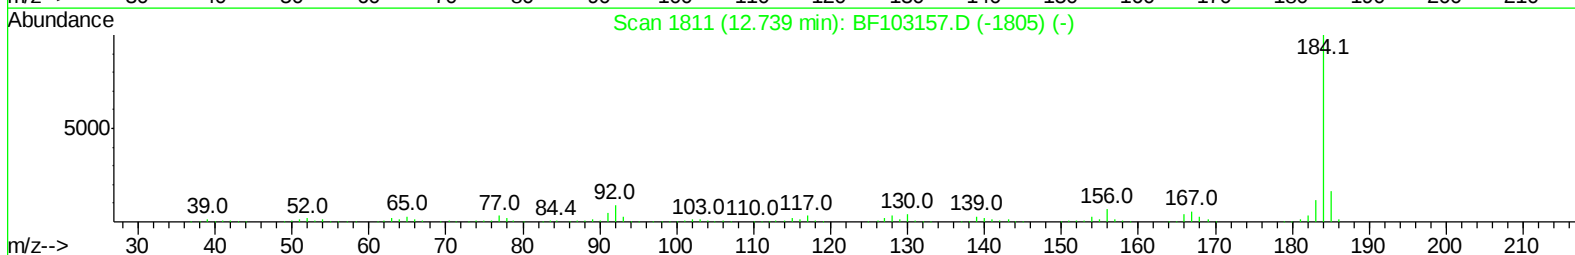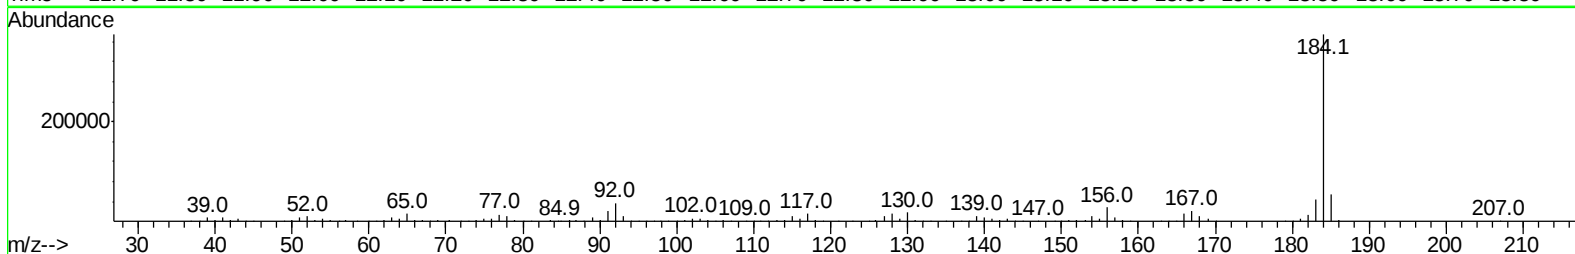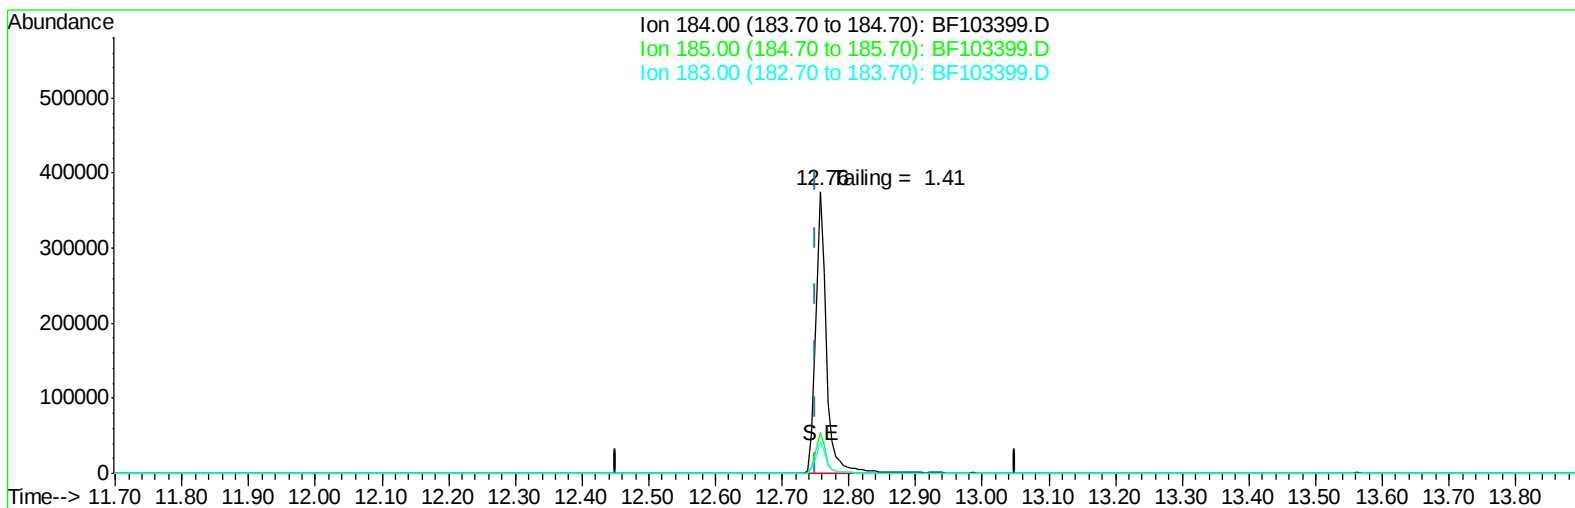

TIC: BF103399.D

(76) Benzidine

12.757min (+0.006) 0.00ng

response 415159

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.36
183.00	11.60	11.59
0.00	0.00	0.00