

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030518\
 Data File : BF103418.D
 Acq On : 5 Mar 2018 19:37
 Operator : SJ/JU
 Sample : J1722-19
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-17

Manual Integrations
 APPROVED

Sohil
 3/6/2018 4:23:13 PM

Quant Time: Mar 06 00:33:44 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 05 13:40:47 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	147763	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	613209	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	260715	20.00	ng	0.00
63) Phenanthrene-d10	11.41	188	378311	20.00	ng	0.00
75) Chrysene-d12	14.07	240	211890	20.00	ng	0.00
86) Perylene-d12	15.59	264	198617	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	1020357	104.44	ng	0.00
7) Phenol-d6	6.52	99	1223704	102.36	ng	0.00
23) Nitrobenzene-d5	7.44	82	766709	71.40	ng	0.00
41) 2,4,6-Tribromophenol	10.72	330	177457	80.41	ng	0.00
44) 2-Fluorobiphenyl	9.23	172	1049199	65.60	ng	0.00
78) Terphenyl-d14	13.00	244	696386	79.00	ng	0.00
Target Compounds						
10) Phenol	6.53	94	93023	6.703	ng	Qvalue # 76
31) Naphthalene	8.17	128	64580	2.151	ng	98
48) Acenaphthylene	9.77	152	86104	3.238	ng	97
49) Dimethylphthalate	9.62	163	95806	4.581	ng	98
51) Acenaphthene	9.95	154	50387	3.249	ng	99
54) Dibenzofuran	10.12	168	63184	2.968	ng	97
57) Fluorene	10.46	166	74677	4.118	ng	95
70) Phenanthrene	11.44	178	1090872	52.396	ng	99
71) Anthracene	11.49	178	332058	15.554	ng	100
72) Carbazole	11.65	167	110331	5.190	ng	98
74) Fluoranthene	12.64	202	1488336	71.139	ng	98
77) Pvrene	12.87	202	1300899	78.746	ng	99
80) Benzo(a)anthracene	14.06	228	630198m	45.839	ng	
82) Chrysene	14.10	228	634273m	47.514	ng	
83) Bis(2-ethylhexyl)phthalate	14.02	149	25791	2.190	ng	# 94
85) Indeno(1,2,3-cd)pyrene	17.14	276	246318	23.307	ng	95
87) Benzo(b)fluoranthene	15.15	252	655302m	50.181	ng	
88) Benzo(k)fluoranthene	15.17	252	255552m	20.782	ng	
89) Benzo(a)pvrene	15.53	252	453988	38.930	ng	95
90) Dibenzo(a,h)anthracene	17.14	278	70005	7.769	ng	# 86
91) Benzo(g,h,i)perylene	17.62	276	229648	26.076	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF030518\
Data File : BF103418.D
Acq On : 5 Mar 2018 19:37
Operator : SJ/JU
Sample : J1722-19
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-17

Manual Integrations
APPROVED

Sohil
3/6/2018 4:23:13 PM

Quant Time: Mar 06 00:33:44 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF022218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 05 13:40:47 2018
Response via : Initial Calibration

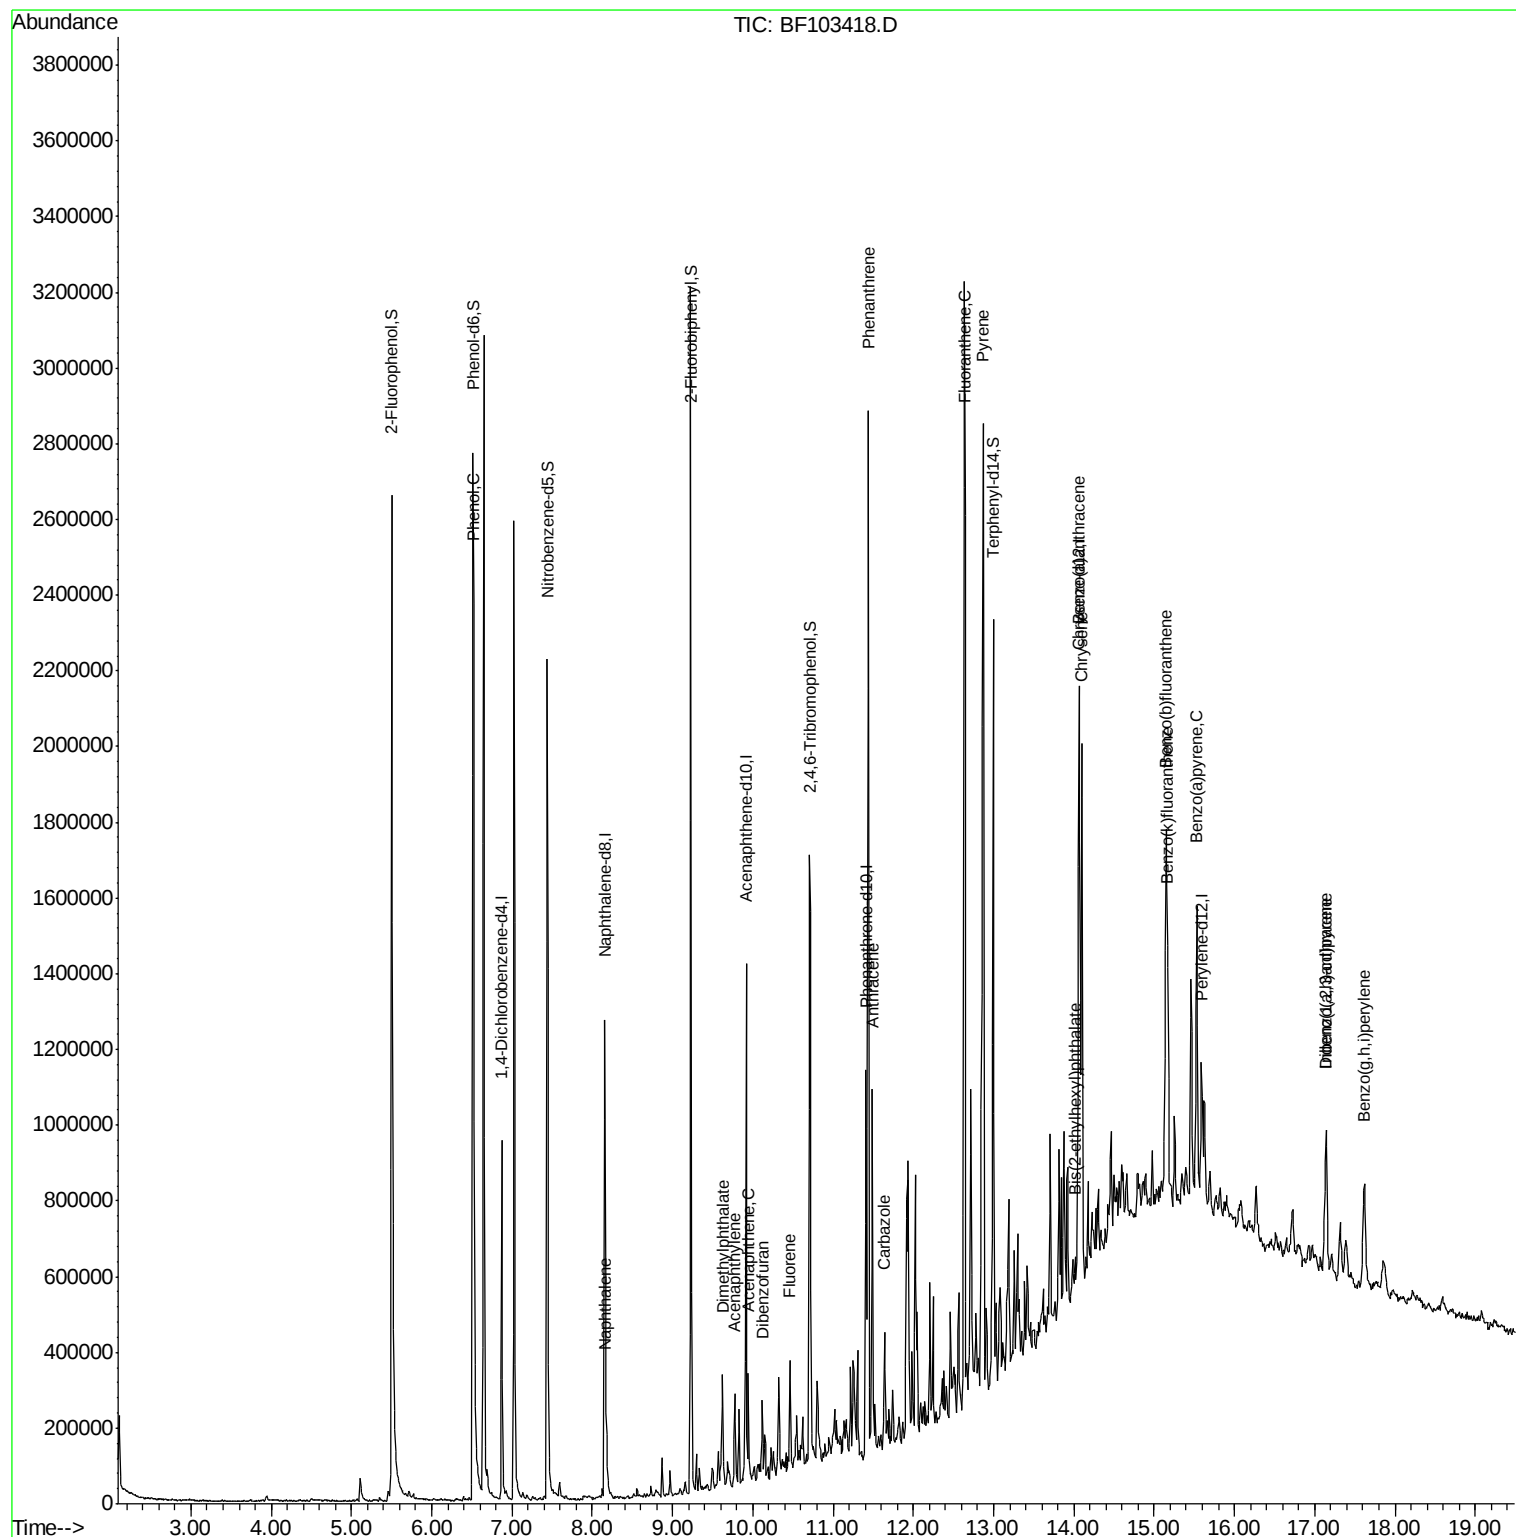



#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.87 min Scan# 813
Delta R.T. 0.00 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Instrument :
BNA_F
ClientSampleId :
SP-17

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.8	124.6	186.8
115	69.7	50.1	75.1

Manual Integrations
APPROVED




Sohil
3/6/2018 4:23:13 PM

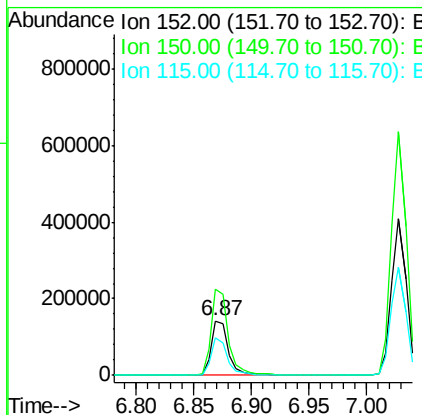


#5

2-Fluorophenol
Concen: 104.439 ng
RT: 5.50 min Scan# 581
Delta R.T. 0.00 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Tgt Ion	Ratio	Lower	Upper
112	100		
64	63.8	47.9	71.9
63	33.5	23.7	35.5

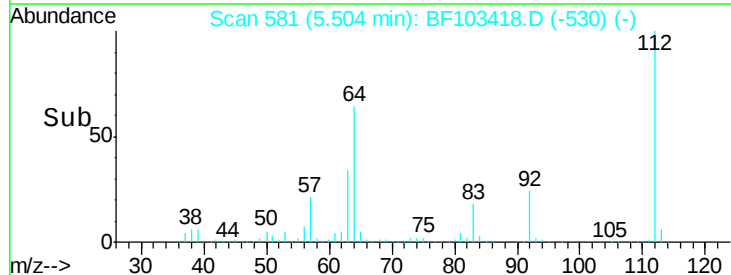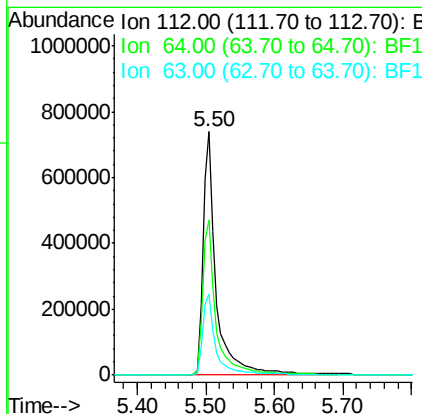

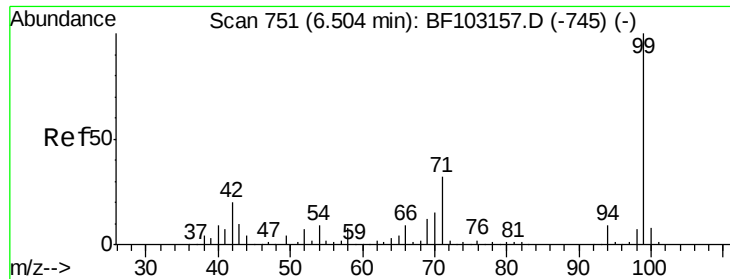

#7

Phenol-d6

Concen: 102.360 ng

RT: 6.52 min Scan# 753

Delta R.T. -0.01 min

Lab File: BF103418.D

Acq: 5 Mar 2018 19:37

Instrument :

BNA_F

ClientSampleId :

SP-17

Tot Ion: 99 Resp: 1223704

Ion Ratio Lower Upper


99 100

42 21.3 14.5 21.7




71 33.6 25.4 38.0

Manual Integrations
APPROVED

Sohil
3/6/2018 4:23:13 PM

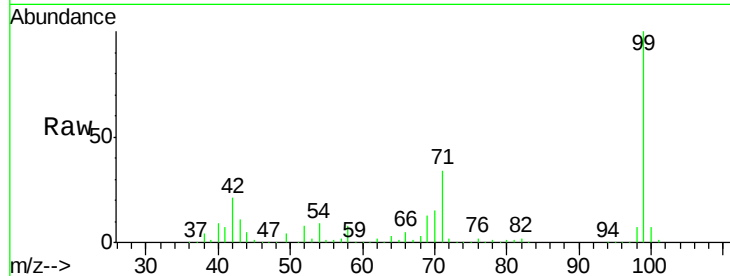

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

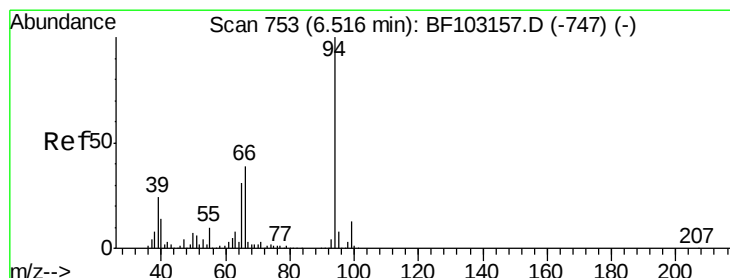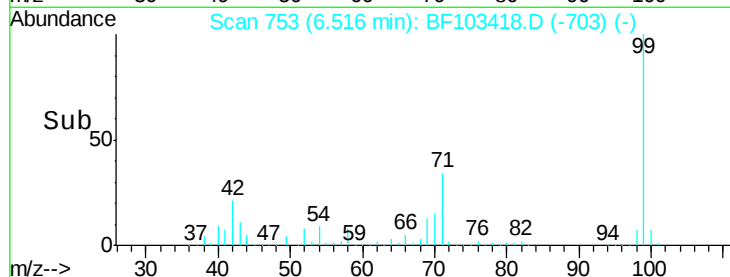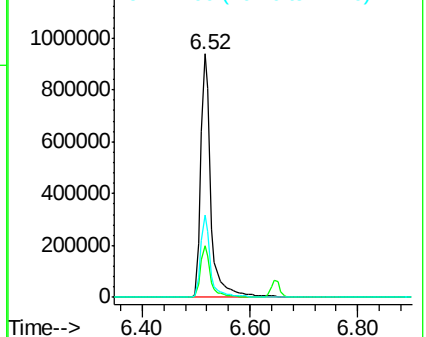

#10

Phenol

Concen: 6.703 ng

RT: 6.53 min Scan# 755

Delta R.T. -0.01 min

Lab File: BF103418.D

Acq: 5 Mar 2018 19:37


Tgt Ion: 94 Resp: 93023

Ion Ratio Lower Upper



94 100

65 32.9 7.9 47.9

66 57.2 16.2 56.2#

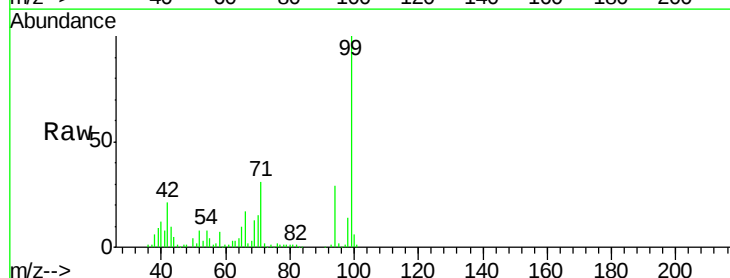

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

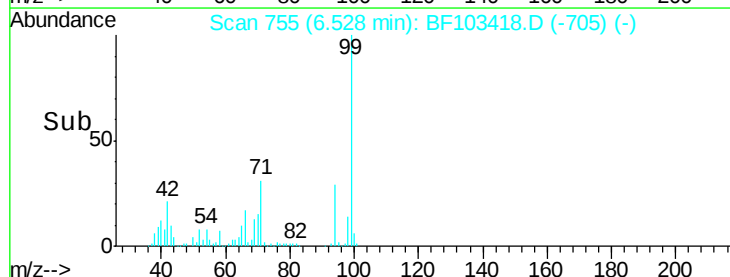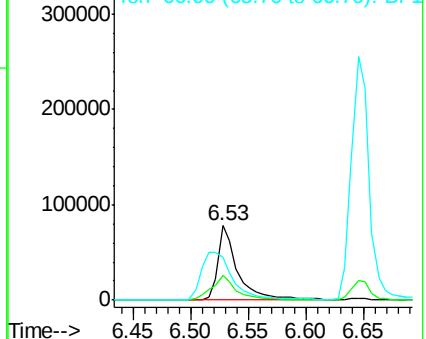




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.16 min Scan# 1032
Delta R.T. 0.00 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Instrument :
BNA_F
ClientSampled :
SP-17




Tot Ion	Ion	Ratio	Resp	Lower	Upper
136	100		613209		
137	10.8		8.9	13.3	
54	9.2		6.6	9.8	
68	6.4		5.0	7.4	

Manual Integrations
APPROVED

Sohil
3/6/2018 4:23:13 PM




Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

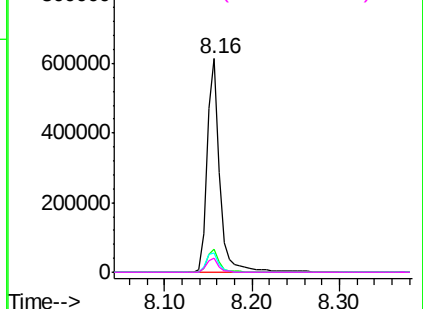




#23
Nitrobenzene-d5
Concen: 71.404 ng
RT: 7.44 min Scan# 910
Delta R.T. 0.00 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
82	100		766709		
128	42.9		36.1	54.1	
54	60.5		41.4	62.2	



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

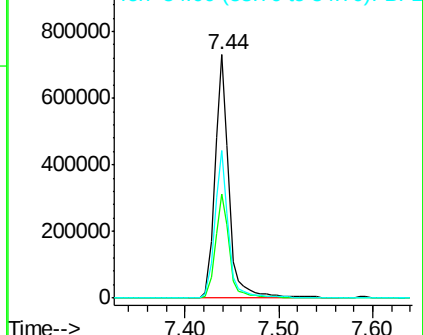

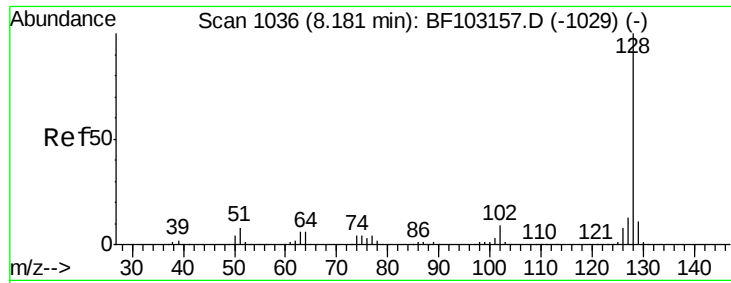


#31
Naphthalene
Concen: 2.151 ng
RT: 8.17 min Scan# 1035
Delta R.T. -0.01 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Instrument :
BNA_F
ClientSampled :
SP-17

Tot Ion	Ratio	Lower	Upper
128	100		
129	11.7	8.8	13.2
127	14.1	10.9	16.3

Manual Integrations
APPROVED

Sohil
3/6/2018 4:23:13 PM






Abundance

Ion 128.00 (127.70 to 128.70): E


Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

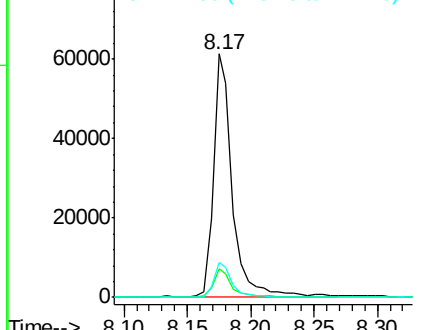

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.92 min Scan# 1331
Delta R.T. 0.00 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.4	86.1	129.1
160	47.0	38.3	57.5






Abundance

Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

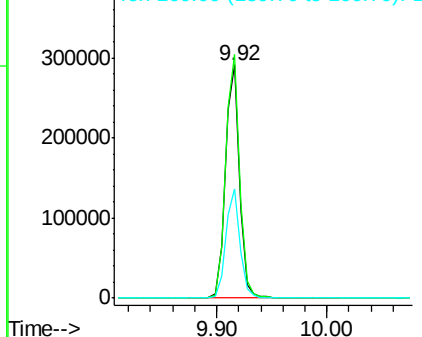

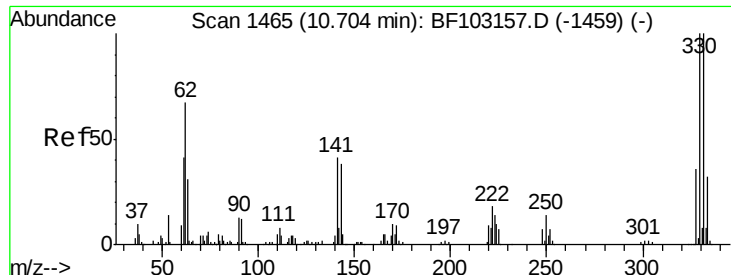


#41
 2,4,6-Tribromophenol
 Concen: 80.413 ng
 RT: 10.72 min Scan# 1467
 Delta R.T. 0.00 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37

Instrument :
 BNA_F
 ClientSampled :
 SP-17

Tot Ion	Ratio	Lower	Upper
330	100		
332	101.8	77.0	115.6
141	45.6	29.9	44.9

Manual Integrations
 APPROVED

Sohil
 3/6/2018 4:23:13 PM






Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

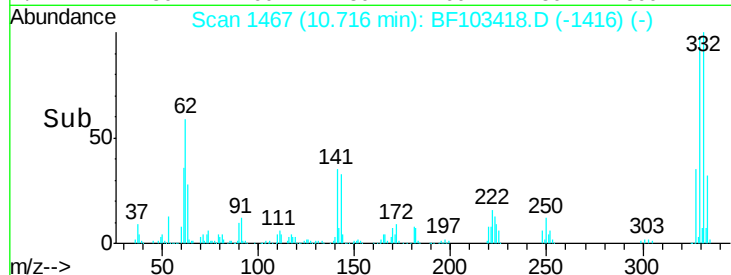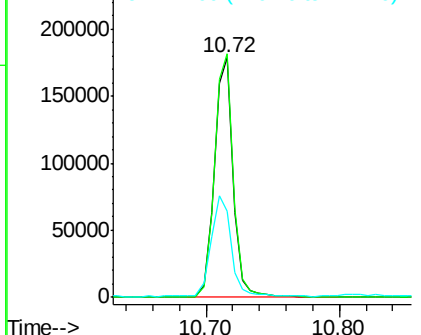

#44
 2-Fluorobiphenyl
 Concen: 65.599 ng
 RT: 9.23 min Scan# 1214
 Delta R.T. -0.01 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37




Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.1	29.7	44.5
170	24.5	19.6	29.4


Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

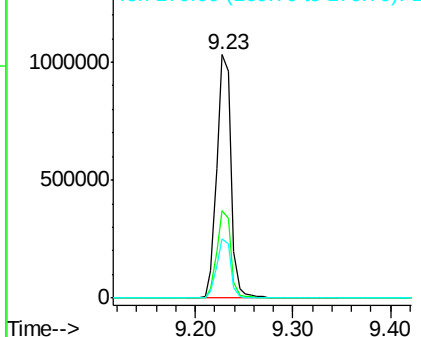



#48

Acenaphthylene

Concen: 3.238 ng

RT: 9.77 min Scan# 1307

Delta R.T. -0.01 min

Lab File: BF103418.D

Acq: 5 Mar 2018 19:37

Instrument :

BNA_F


ClientSampleId :

SP-17




Tot Ion:	152	Resp:	86104
Ion Ratio	Lower	Upper	
152	100		
151	18.4	16.3	24.5
153	12.8	10.7	16.1

Manual Integrations
APPROVED

Sohil
3/6/2018 4:23:13 PM



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

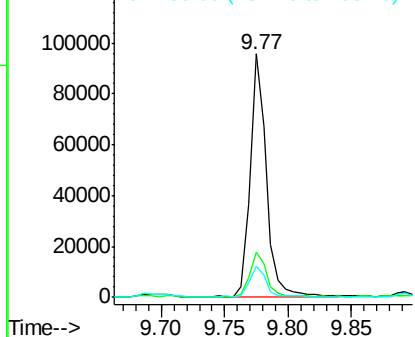

#49

Dimethylphthalate

Concen: 4.581 ng


RT: 9.62 min Scan# 1281

Delta R.T. -0.01 min



Lab File: BF103418.D


Acq: 5 Mar 2018 19:37

Tgt Ion:	163	Resp:	95806
Ion Ratio	Lower	Upper	
163	100		
194	3.1	2.7	4.1
164	9.4	8.2	12.2



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

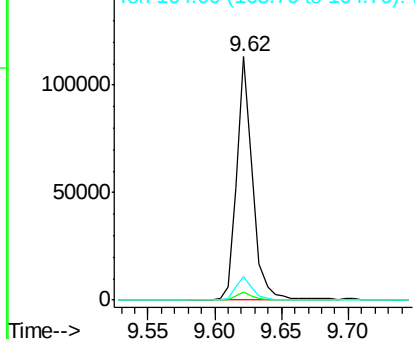



#51

Acenaphthene

Concen: 3.249 ng

RT: 9.95 min Scan# 1336

Delta R.T. -0.01 min

Lab File: BF103418.D

Acq: 5 Mar 2018 19:37

Instrument :

BNA_F


ClientSampleId :

SP-17




Tot Ion:	154	Resp:	50387
Ion	Ratio	Lower	Upper
154	100		
153	113.1	91.2	136.8
152	55.7	43.8	65.8

Manual Integrations
APPROVED

Sohil
3/6/2018 4:23:13 PM



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E

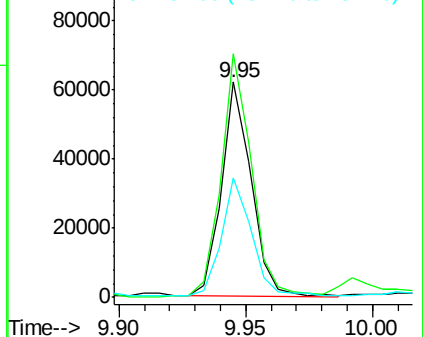

#54

Dibenzofuran

Concen: 2.968 ng

RT: 10.12 min Scan# 1366




Delta R.T. 0.00 min


Lab File: BF103418.D

Acq: 5 Mar 2018 19:37

Tgt Ion:	168	Resp:	63184
Ion	Ratio	Lower	Upper
168	100		
139	39.7	30.1	45.1
169	14.3	10.9	16.3

Abundance Ion 168.00 (167.70 to 168.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 169.00 (168.70 to 169.70): E

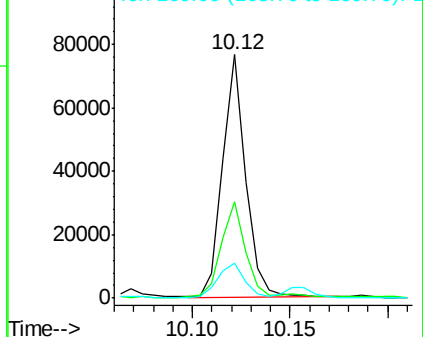







#57
Fluorene
 Concen: 4.118 ng
 RT: 10.46 min Scan# 1424
 Delta R.T. -0.01 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37

Instrument :
 BNA_F
 ClientSampled :
 SP-17

Tot Ion	Ratio	Lower	Upper
166	100		
165	95.1	79.8	119.8
167	15.2	10.6	16.0




Manual Integrations
 APPROVED


Sohil
 3/6/2018 4:23:13 PM

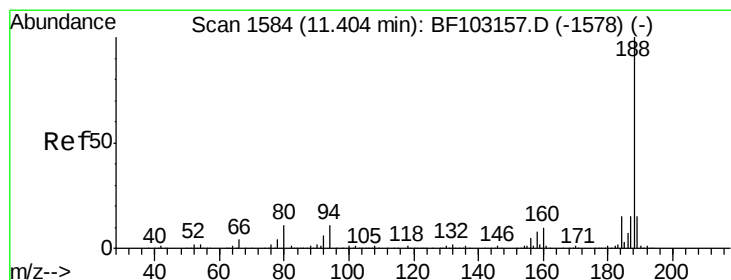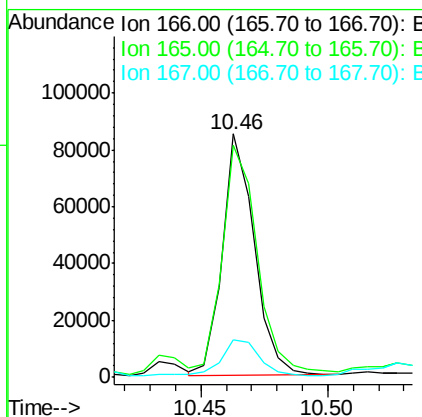

#63
Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.41 min Scan# 1585
 Delta R.T. 0.00 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37

Tgt Ion	Ratio	Lower	Upper
188	100		
94	11.9	8.5	12.7
80	13.7	9.2	13.8

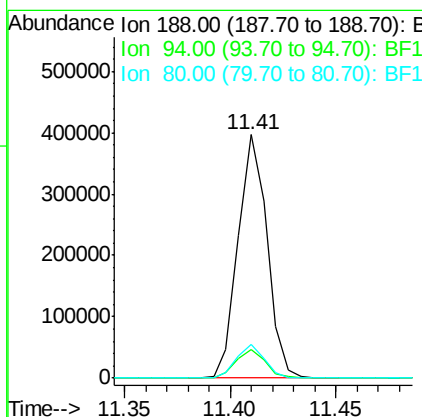




#70
Phenanthrene
Concen: 52.396 ng
RT: 11.44 min Scan# 1590
Delta R.T. 0.01 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Instrument :
BNA_F
ClientSampled :
SP-17




Tot Ion:178 Resp: 1090872
Ion Ratio Lower Upper
178 100
176 19.9 15.8 23.8
179 15.9 13.0 19.6

Manual Integrations
APPROVED

Sohil
3/6/2018 4:23:13 PM






Abundance Ion 178.00 (177.70 to 178.70): E
1500000 Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

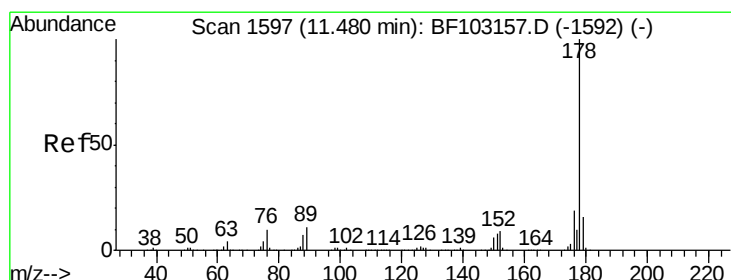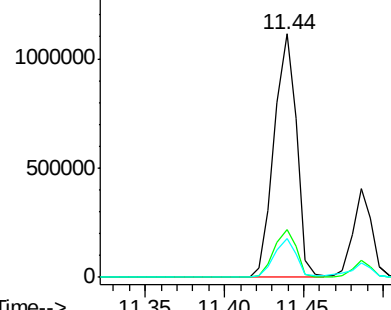


#71
Anthracene
Concen: 15.554 ng
RT: 11.49 min Scan# 1598
Delta R.T. 0.00 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Tgt Ion:178 Resp: 332058
Ion Ratio Lower Upper
178 100
176 19.1 15.4 23.2
179 15.8 12.6 19.0

Abundance Ion 178.00 (177.70 to 178.70): E
1500000 Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

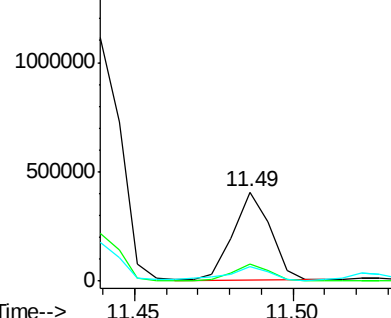







#72
 Carbazole
 Concen: 5.190 ng
 RT: 11.65 min Scan# 1625
 Delta R.T. -0.01 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37

Instrument :
 BNA_F
 ClientSampleId :
 SP-17

Tot Ion	Ion	Ratio	Resp	Lower	Upper
167	100				
166	21.2	17.6	26.4		
139	14.1	10.9	16.3		




Manual Integrations
 APPROVED




Sohil
 3/6/2018 4:23:13 PM

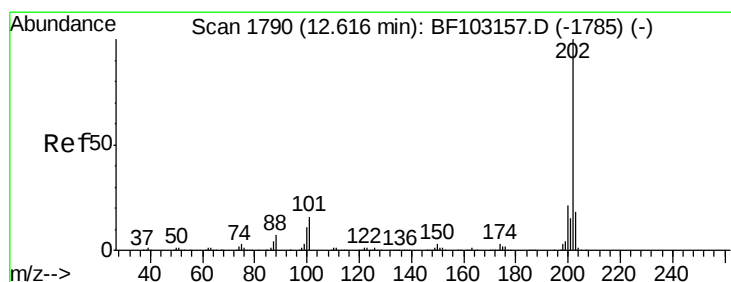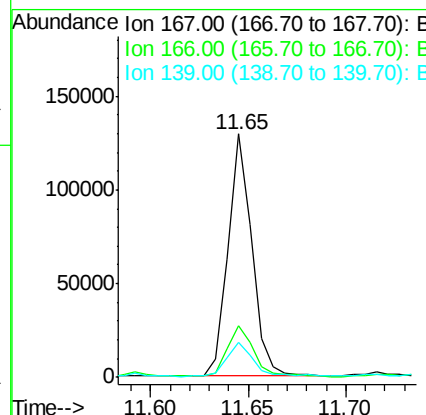

#74
 Fluoranthene
 Concen: 71.139 ng
 RT: 12.64 min Scan# 1794
 Delta R.T. 0.01 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37

Tgt Ion	Ion	Ratio	Resp	Lower	Upper
202	100				
101	15.4	0.0	34.1		
203	17.7	0.0	38.1		

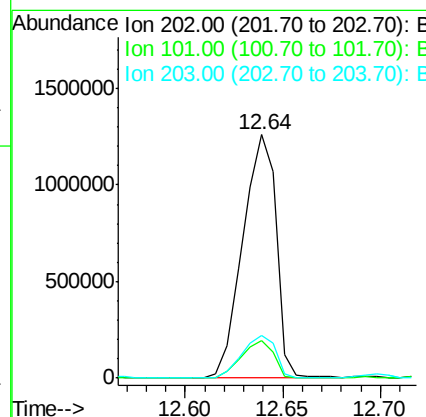







#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.07 min Scan# 2038
Delta R.T. 0.01 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Instrument :
BNA_F
ClientSampleId :
SP-17

Tot Ion	Ratio	Lower	Upper
240	100		
120	14.3	9.5	14.3
236	26.6	20.7	31.1


Manual Integrations
APPROVED


Sohil
3/6/2018 4:23:13 PM

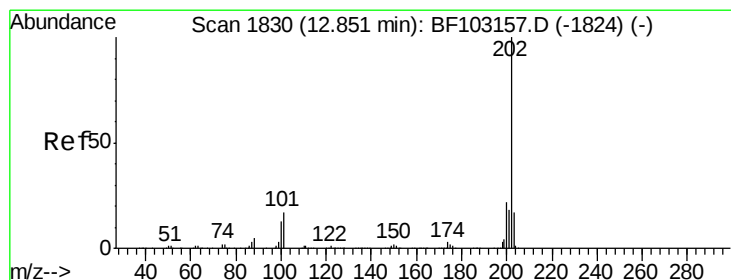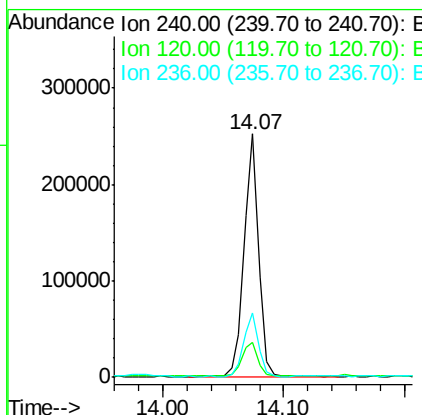

#77
Pyrene
Concen: 78.746 ng
RT: 12.87 min Scan# 1834
Delta R.T. 0.01 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Tgt Ion	Ratio	Lower	Upper
202	100		
200	22.0	17.4	26.2
203	18.2	14.3	21.5

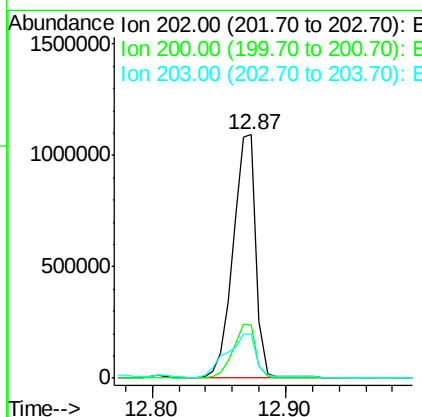

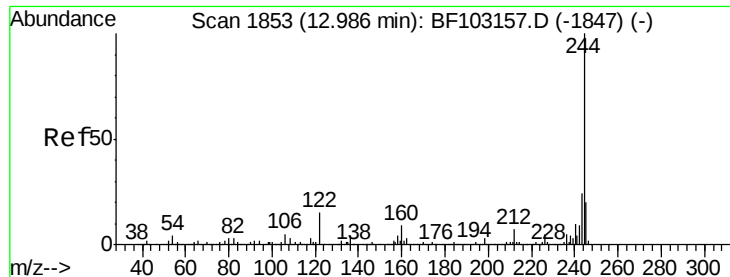





#78
 Terphenyl-d14
 Concen: 79.004 ng
 RT: 13.00 min Scan# 1855
 Delta R.T. 0.01 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37

Instrument :
 BNA_F
 ClientSampled :
 SP-17

Tot Ion	Ratio	Lower	Upper
244	100		
212	6.9	5.4	8.0
122	13.8	11.0	16.4




Manual Integrations
 APPROVED


Sohil
 3/6/2018 4:23:13 PM

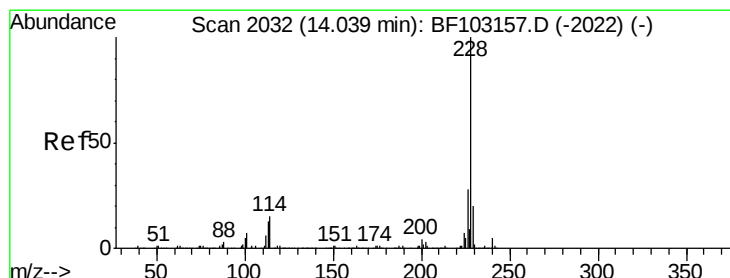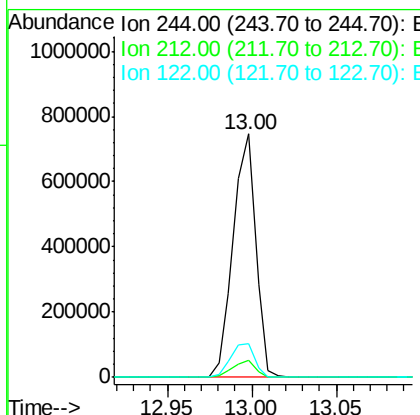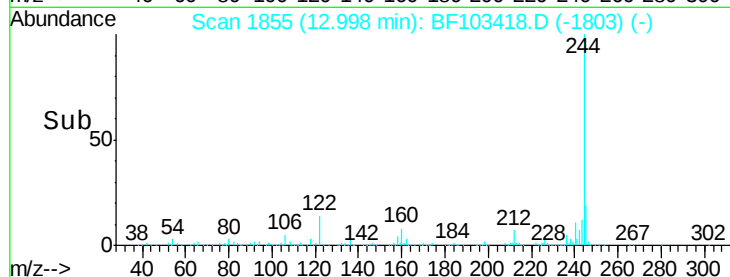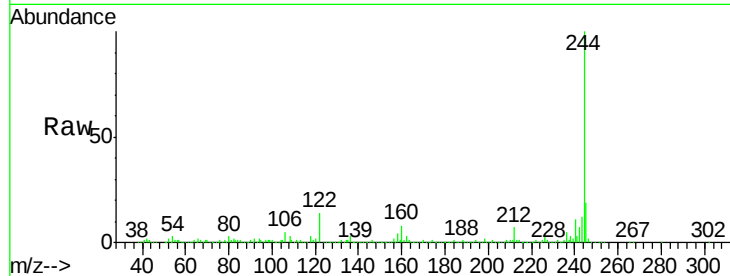

#80
 Benzo(a)anthracene
 Concen: 45.839 ng m
 RT: 14.06 min Scan# 2036
 Delta R.T. 0.01 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.1	22.6	33.8
229	20.5	15.8	23.6

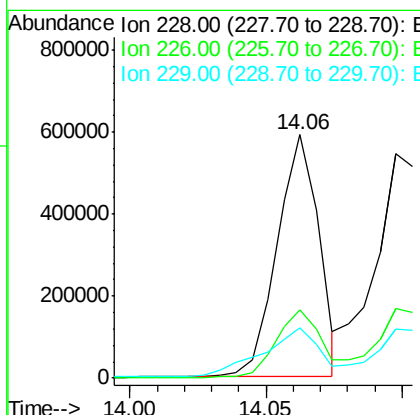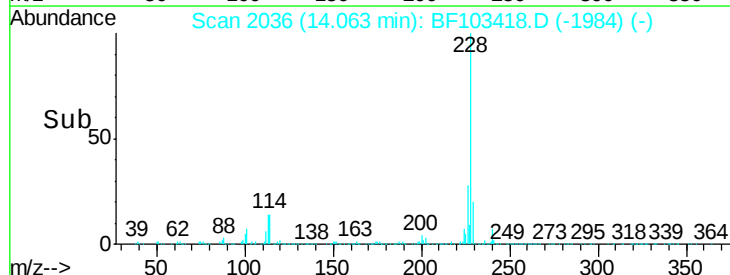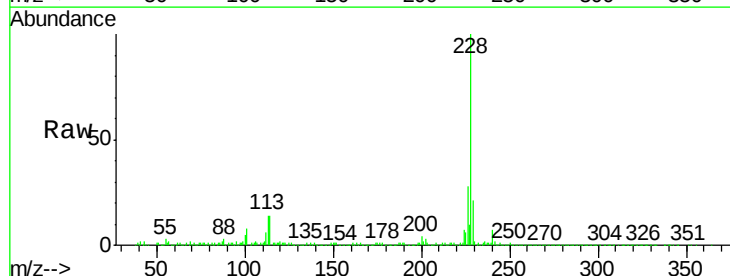







#82
 Chrvsene
 Concen: 47.514 ng/ml
 RT: 14.10 min Scan# 2042
 Delta R.T. 0.00 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37

Instrument :
 BNA_F
 ClientSampleId :
 SP-17

Tot Ion	Ratio	Lower	Upper
228	100		
226	30.8	25.0	37.6
229	21.9	16.2	24.4




Manual Integrations
 APPROVED


Sohil
 3/6/2018 4:23:13 PM

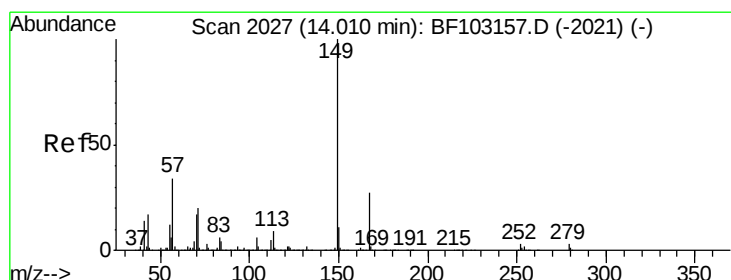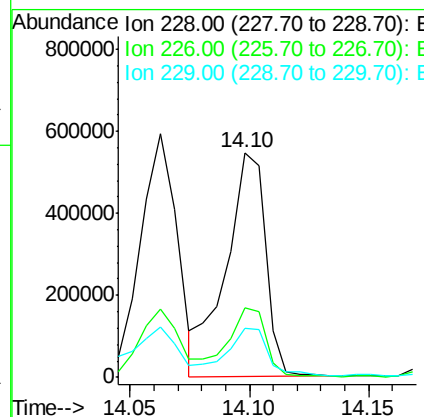

#83
 Bis(2-ethylhexyl)phthalate
 Concen: 2.190 ng
 RT: 14.02 min Scan# 2028
 Delta R.T. 0.00 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37

Tgt Ion	Ratio	Lower	Upper
149	100		
167	30.2	21.3	31.9
279	4.5	3.0	4.4#

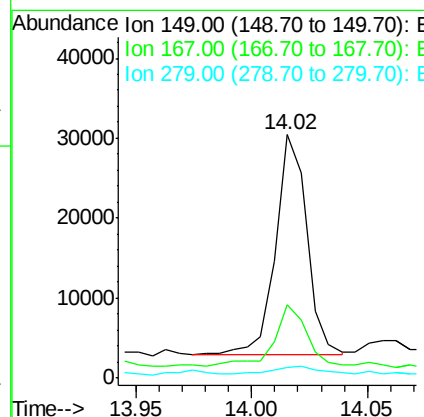







#85
Indeno(1,2,3-cd)pyrene
Concen: 23.307 ng
RT: 17.14 min Scan# 2560
Delta R.T. 0.01 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Instrument :
BNA_F
ClientSampleId :
SP-17

Tot Ion	Ratio	Resp	Lower	Upper
276	100	246318		
138	27.7		25.0	37.6
277	24.1		20.1	30.1




Manual Integrations
APPROVED


Sohil
3/6/2018 4:23:13 PM

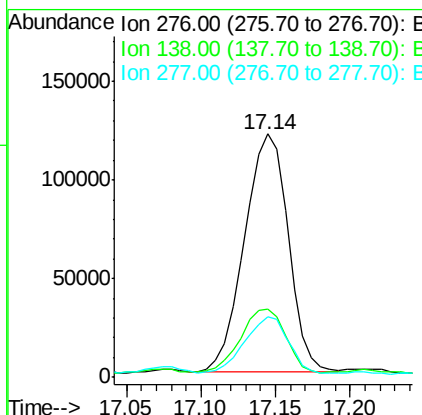

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.59 min Scan# 2296
Delta R.T. 0.02 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Tgt Ion	Ratio	Resp	Lower	Upper
264	100	198617		
260	25.2		19.2	28.8
265	23.9		17.5	26.3

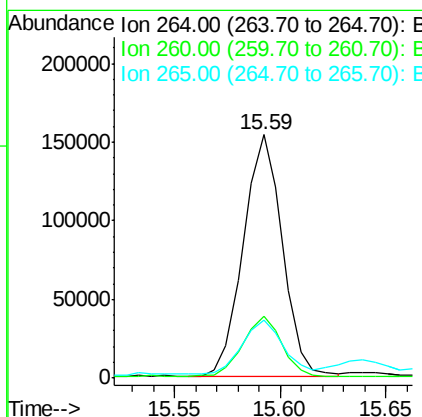







#87
Benzo(b)fluoranthene
Concen: 50.181 ng m
RT: 15.15 min Scan# 2221
Delta R.T. 0.02 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Instrument :
BNA_F
ClientSampled :
SP-17

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.0	17.0	25.6
125	15.6	9.0	13.6




Manual Integrations
APPROVED


Sohil
3/6/2018 4:23:13 PM

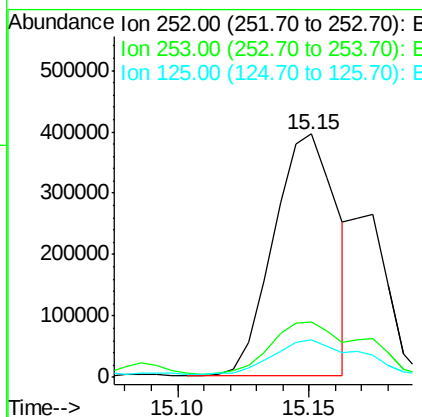

#88
Benzo(k)fluoranthene
Concen: 20.782 ng m
RT: 15.17 min Scan# 2225
Delta R.T. 0.01 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.1	17.9	26.9
125	13.7	10.2	15.2

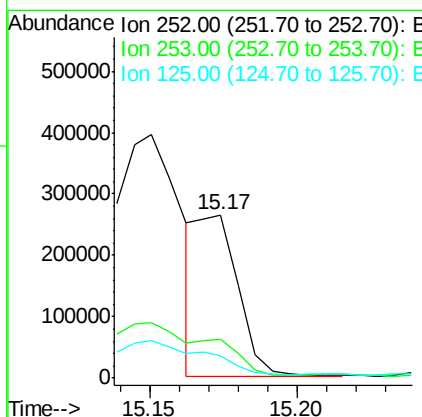

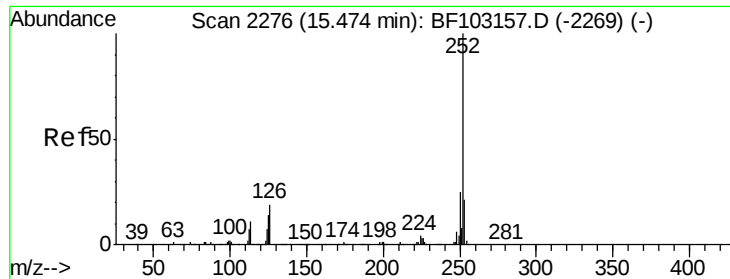





#89
Benzo(a)pyrene
Concen: 38.930 ng
RT: 15.53 min Scan# 2286
Delta R.T. 0.02 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Instrument :
BNA_F
ClientSampled :
SP-17

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.6	17.1	25.7
125	13.9	9.8	14.6




Manual Integrations
APPROVED




Sohil
3/6/2018 4:23:13 PM

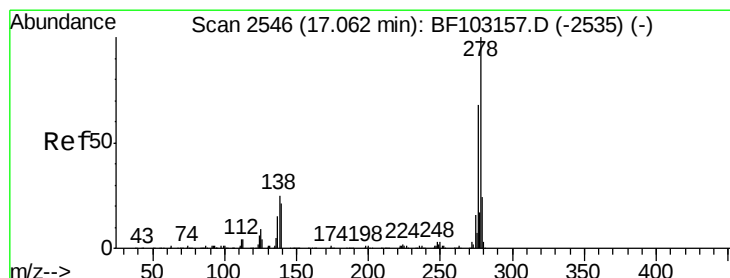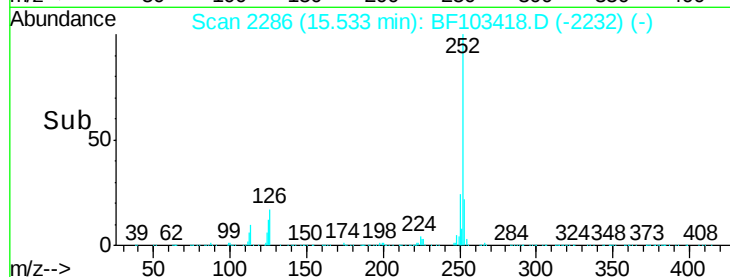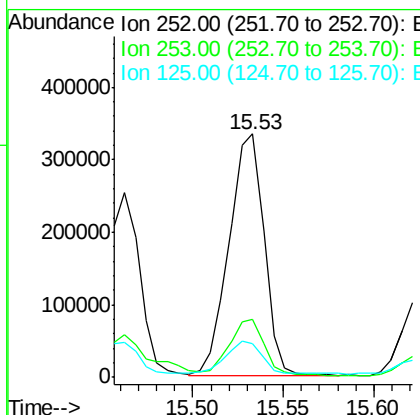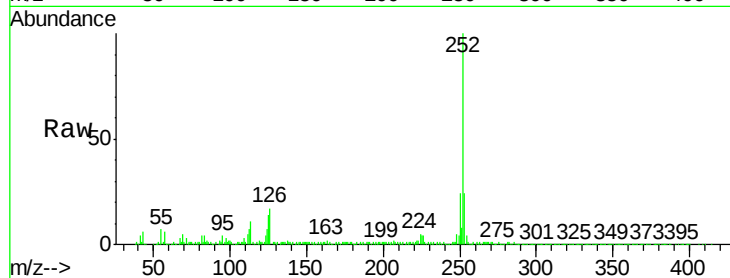

#90
Dibenzo(a,h)anthracene
Concen: 7.769 ng
RT: 17.14 min Scan# 2560
Delta R.T. 0.01 min
Lab File: BF103418.D
Acq: 5 Mar 2018 19:37

Tgt Ion	Ratio	Lower	Upper
278	100		
139	29.4	15.9	23.9#
279	27.9	19.0	28.4

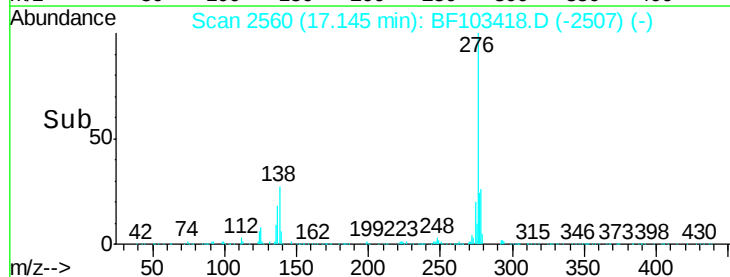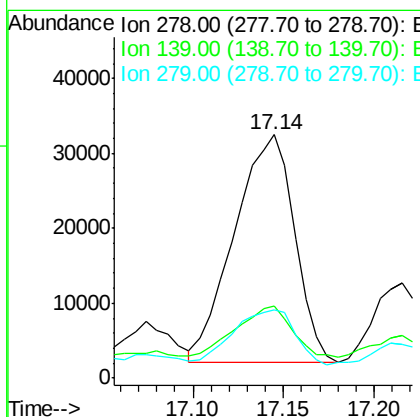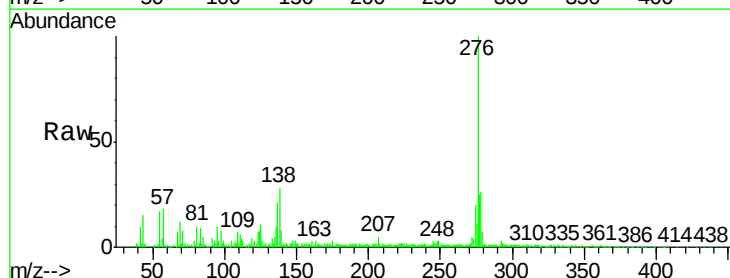



#91
 Benzo(a,h,i)perylene
 Concen: 26.076 ng
 RT: 17.62 min Scan# 2641
 Delta R.T. 0.03 min
 Lab File: BF103418.D
 Acq: 5 Mar 2018 19:37

Instrument :
 BNA_F
 ClientSampleId :
 SP-17

Tot Ion	Ratio	Lower	Upper
276	100		
277	24.2	17.9	26.9
138	29.8	21.8	32.8

Manual Integrations
 APPROVED

Sohil
 3/6/2018 4:23:13 PM

