


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030518\
Data File : BF103399.D
Acq On : 5 Mar 2018 10:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 05 13:40:47 2018

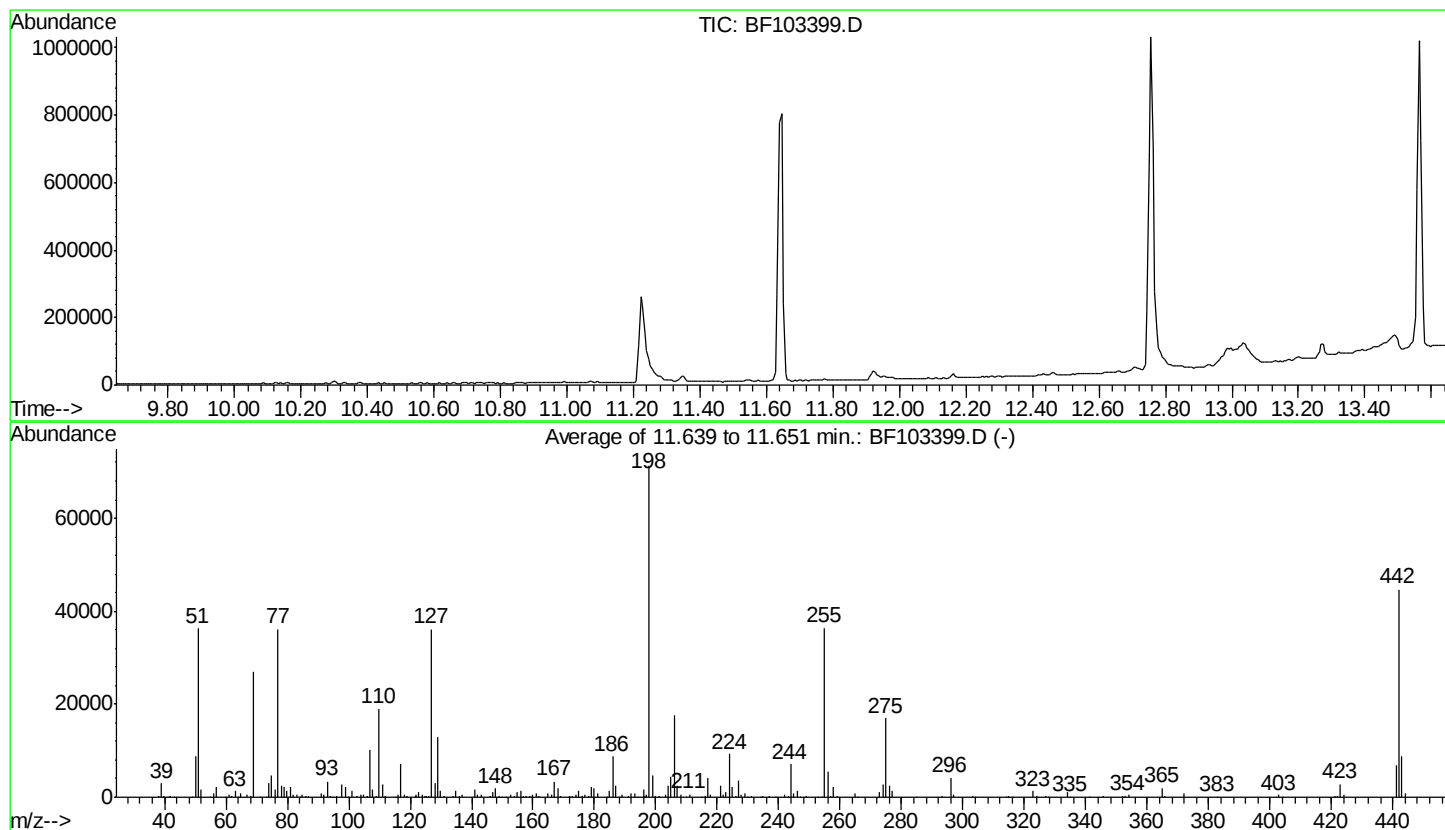

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.9	36288	PASS
68	69	0.00	2	1.5	405	PASS
69	198	0.00	100	37.8	26955	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.6	36089	PASS
197	198	0.00	2	0.6	447	PASS
198	198	100	100	100.0	71301	PASS
199	198	5	9	6.7	4808	PASS
275	198	10	60	23.9	17030	PASS
365	198	1	100	2.8	1996	PASS
441	443	0.01	100	76.5	6845	PASS
442	198	50	100	62.6	44610	PASS
443	442	15	24	20.1	8949	PASS