


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF030518\
 Data File : BF103413.D
 Acq On : 5 Mar 2018 17:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF022218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 05 13:40:47 2018

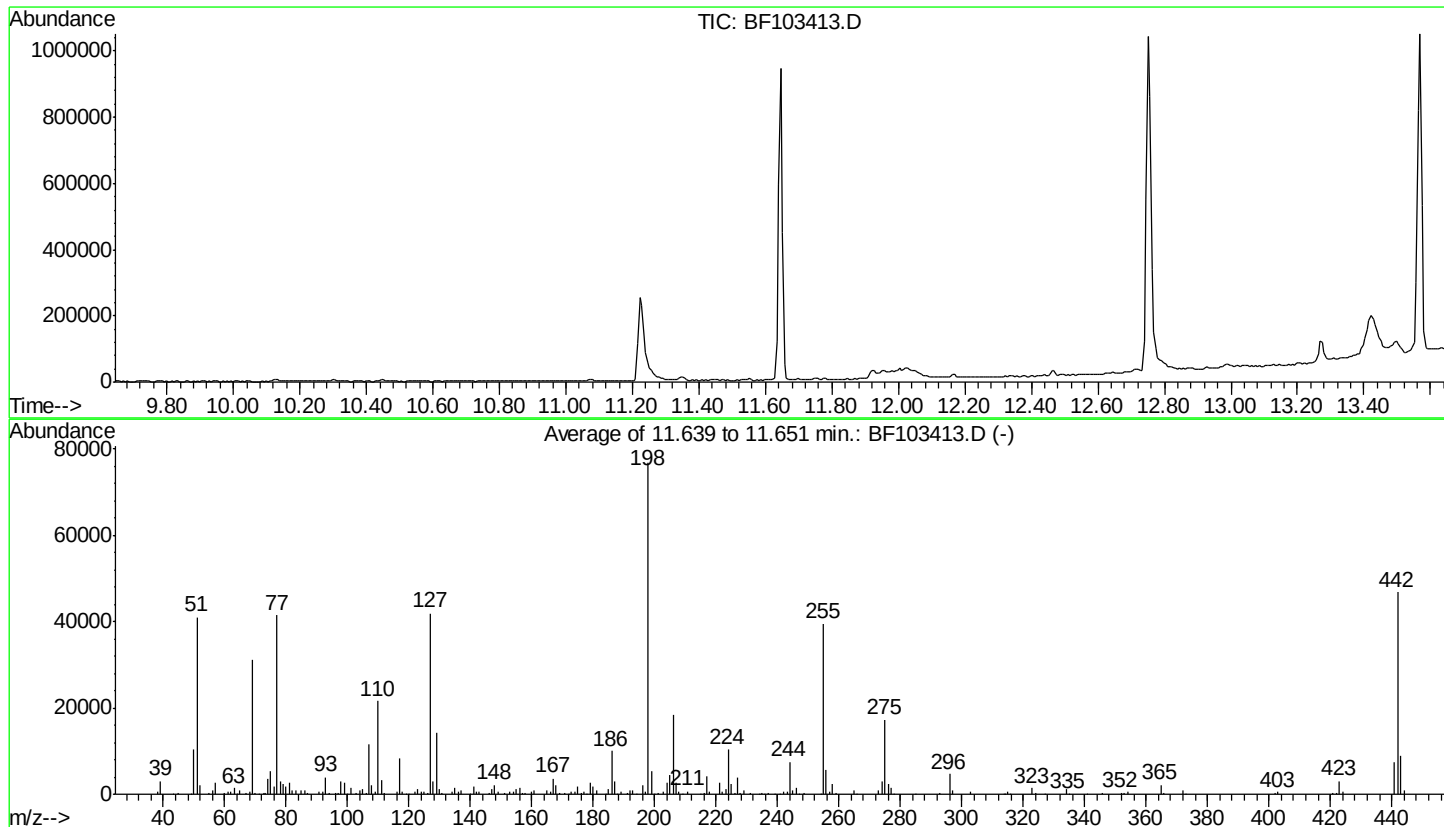

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.4	41008	PASS
68	69	0.00	2	1.6	505	PASS
69	198	0.00	100	40.6	31149	PASS
70	69	0.00	2	0.7	230	PASS
127	198	10	80	54.5	41818	PASS
197	198	0.00	2	0.7	559	PASS
198	198	100	100	100.0	76760	PASS
199	198	5	9	6.8	5199	PASS
275	198	10	60	22.6	17317	PASS
365	198	1	100	2.9	2198	PASS
441	443	0.01	100	84.5	7449	PASS
442	198	50	100	60.9	46768	PASS
443	442	15	24	18.8	8815	PASS